

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110321\
 Data File : VY006610.D
 Acq On : 03 Nov 2021 18:41
 Operator : SY/MD
 Sample : M4472-07
 Misc : 5.01G/5ML/MSVOA_Y/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-2-KD

Quant Time: Nov 03 21:23:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y102221S.M
 Quant Title : SW846 8260
 QLast Update : Sat Oct 23 06:59:04 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.801	168	72382	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	120496	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.495	117	108434	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	40363	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.148	65	52026	58.410	ug/l	0.00
Spiked Amount	50.000	Range 50 - 163	Recovery	=	116.820%	
35) Dibromofluoromethane	7.728	113	37899	56.430	ug/l	0.00
Spiked Amount	50.000	Range 54 - 147	Recovery	=	112.860%	
50) Toluene-d8	10.185	98	152693	53.632	ug/l	0.00
Spiked Amount	50.000	Range 49 - 140	Recovery	=	107.260%	
62) 4-Bromofluorobenzene	12.483	95	45051	46.974	ug/l	0.00
Spiked Amount	50.000	Range 25 - 144	Recovery	=	93.940%	
Target Compounds						
20) Methylene Chloride	4.728	84	9253	8.259	ug/l	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110321\
Data File : VY006610.D
Acq On : 03 Nov 2021 18:41
Operator : SY/MD
Sample : M4472-07
Misc : 5.01G/5ML/MSVOA_Y/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WC-2-KD

Quant Time: Nov 03 21:23:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y102221S.M
Quant Title : SW846 8260
QLast Update : Sat Oct 23 06:59:04 2021
Response via : Initial Calibration




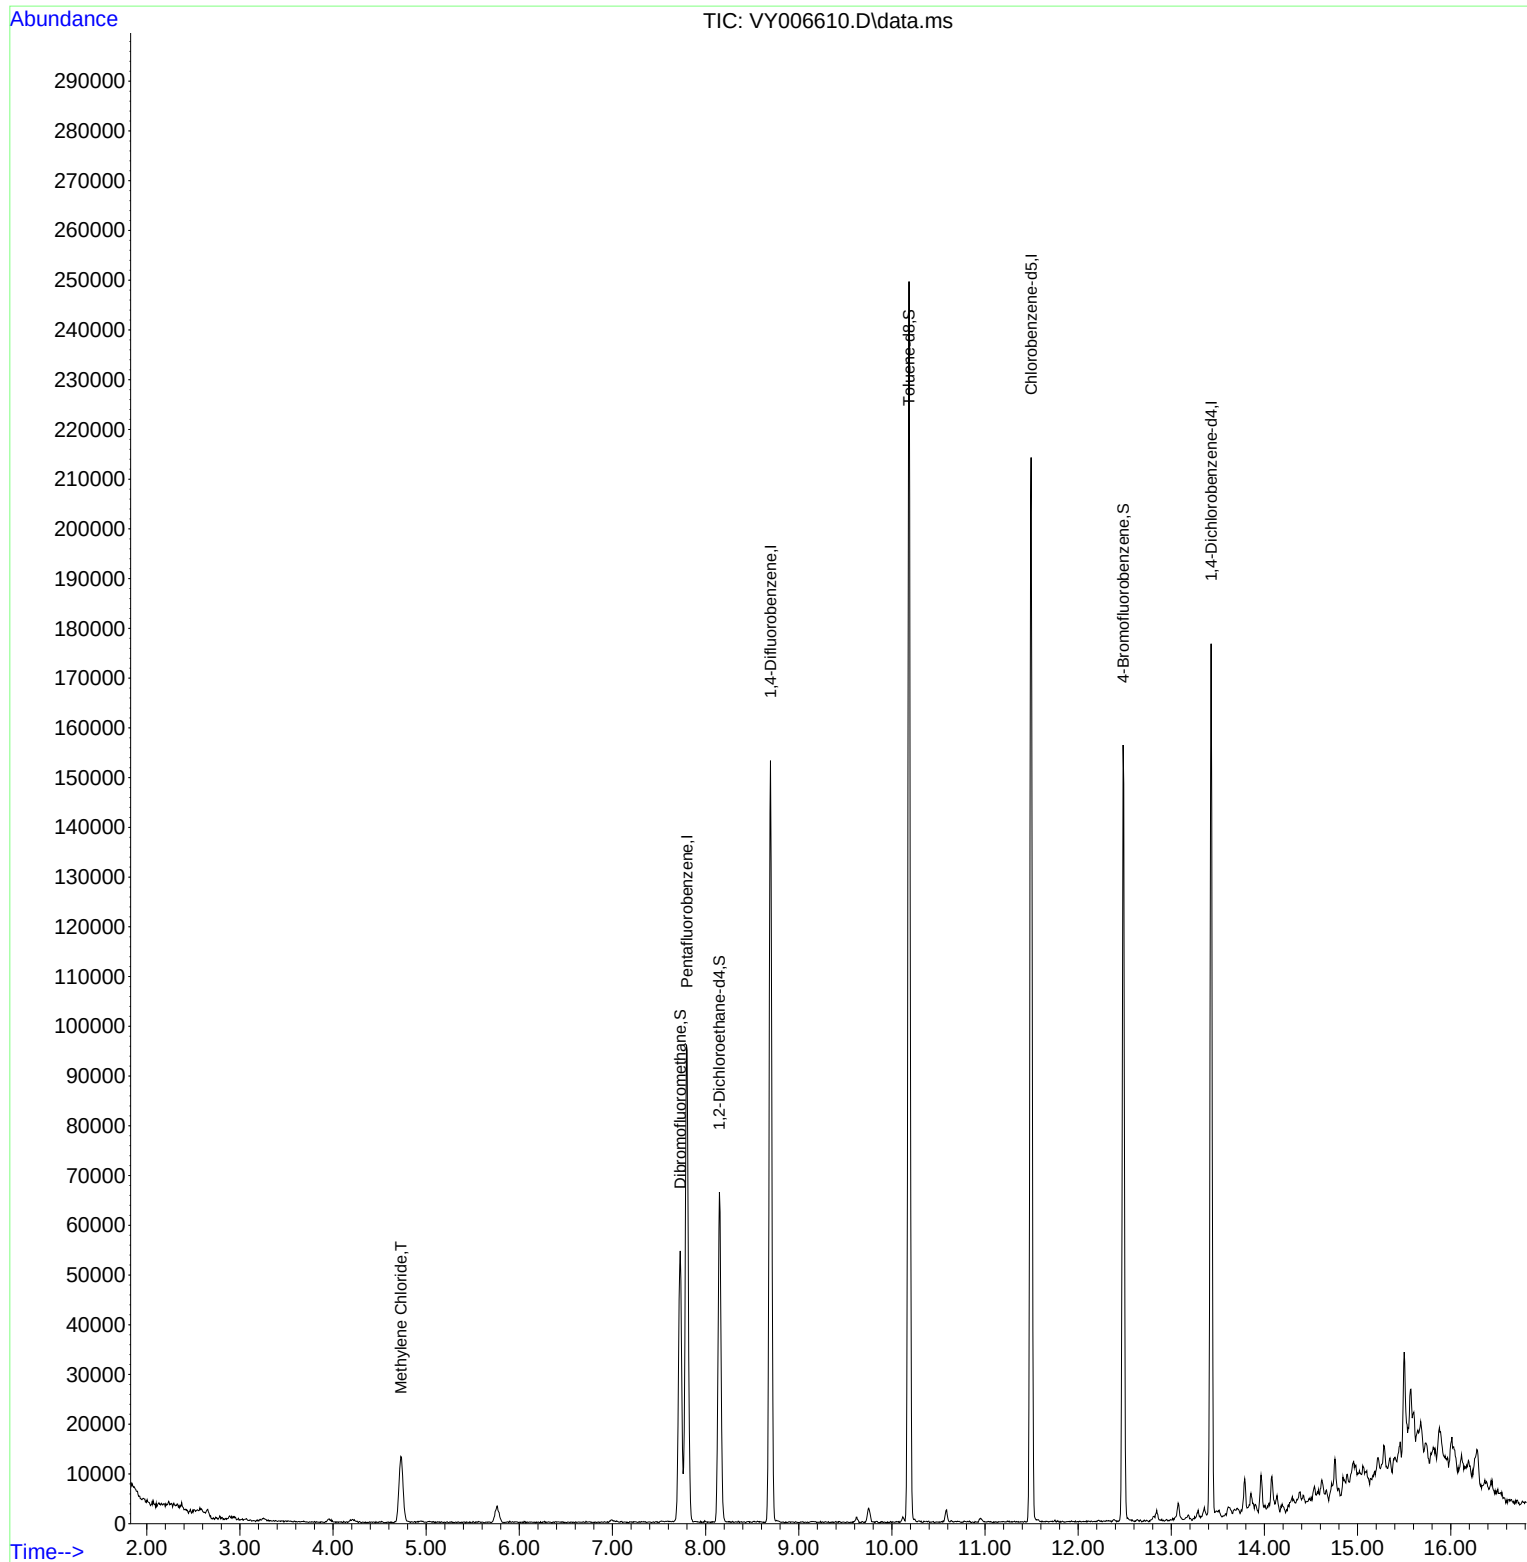


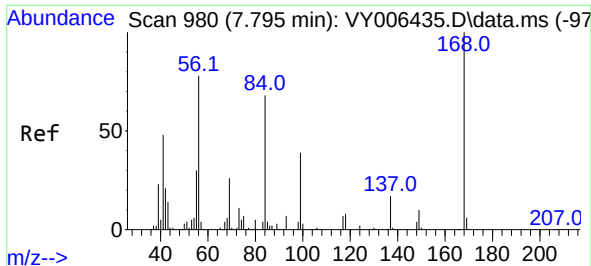

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 980
Delta R.T. 0.006 min
Lab File: VY006610.D
Acq: 03 Nov 2021 18:41




Instrument :
MSVOA_Y
ClientSampleId :
WC-2-KD


Tgt Ion:168 Resp: 72382
Ion Ratio Lower Upper
168 100
99 54.6 44.8 67.2

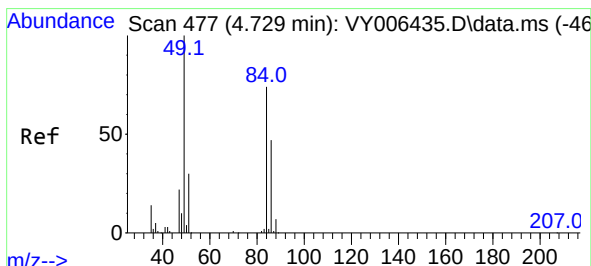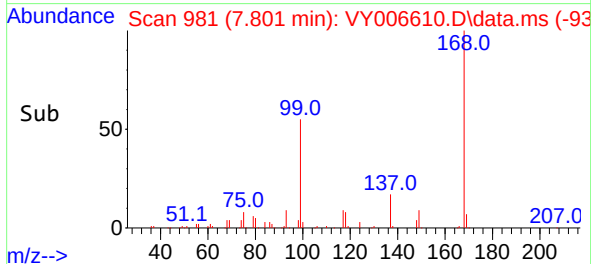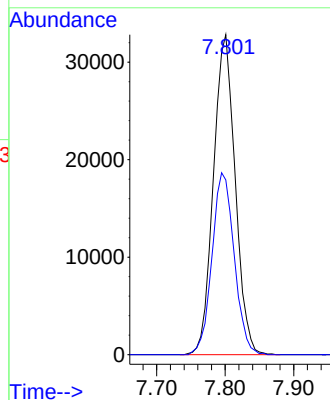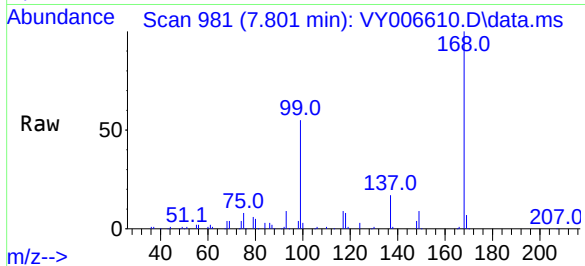

#20
Methylene Chloride
Concen: 8.259 ug/l
RT: 4.728 min Scan# 477
Delta R.T. -0.001 min
Lab File: VY006610.D
Acq: 03 Nov 2021 18:41

Tgt Ion: 84 Resp: 9253
Ion Ratio Lower Upper
84 100
49 139.4 107.8 161.8
51 45.1 32.8 49.2
86 57.9 50.6 75.8

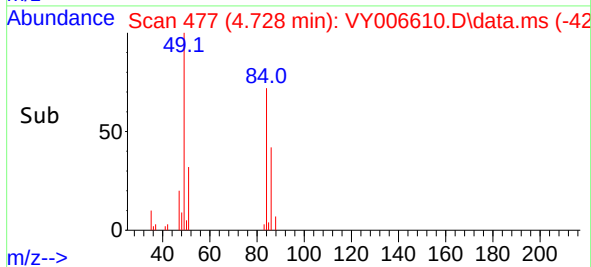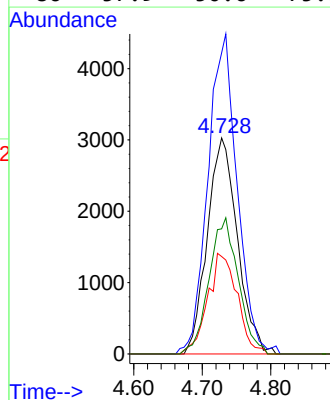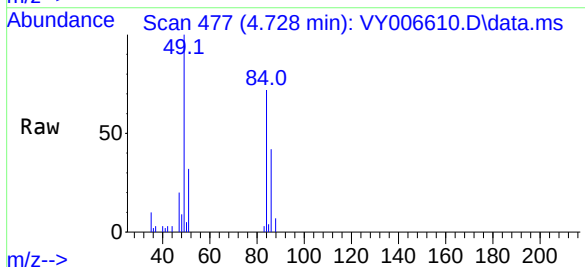

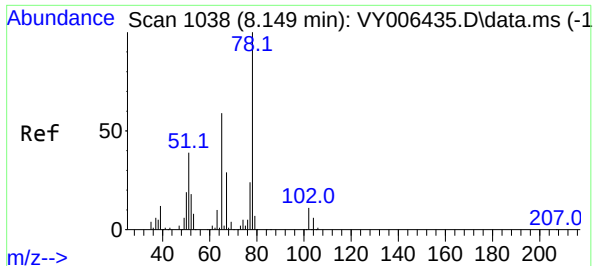

#33

1,2-Dichloroethane-d4

Concen: 58.410 ug/l

RT: 8.148 min Scan# 1103

Delta R.T. -0.000 min

Lab File: VY006610.D

Acq: 03 Nov 2021 18:41

Instrument :

MSVOA_Y

ClientSampleId :





WC-2-KD

Tgt Ion: 65 Resp: 52026

Ion Ratio Lower Upper

65 100

67 52.5 0.0 98.2

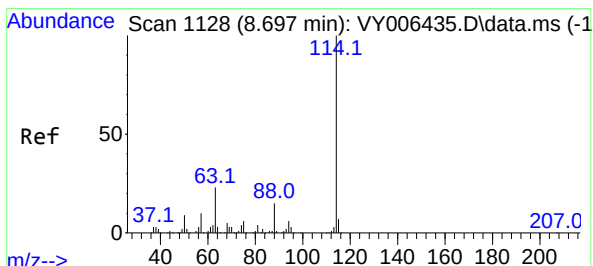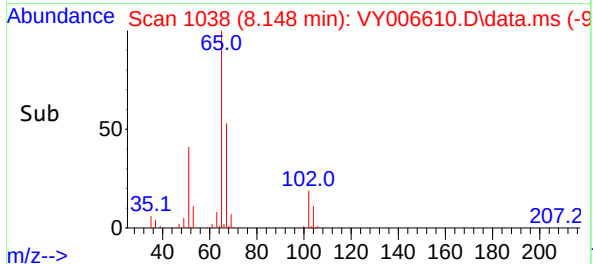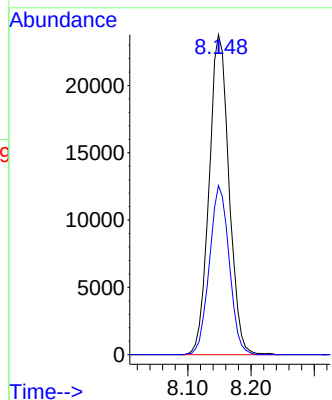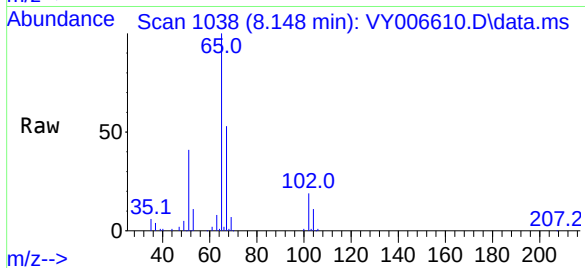

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.697 min Scan# 1128

Delta R.T. -0.000 min

Lab File: VY006610.D

Acq: 03 Nov 2021 18:41




Tgt Ion: 114 Resp: 120496


Ion Ratio Lower Upper

114 100

63 23.6 0.0 45.0

88 15.5 0.0 30.6


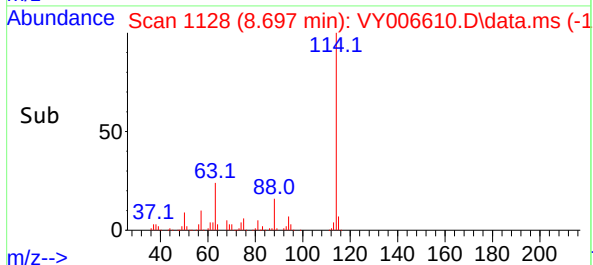
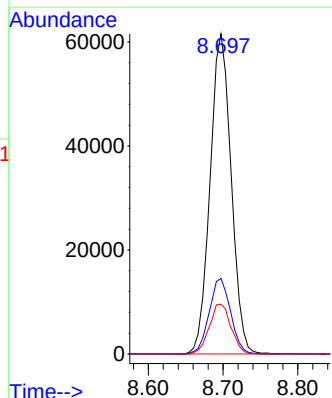
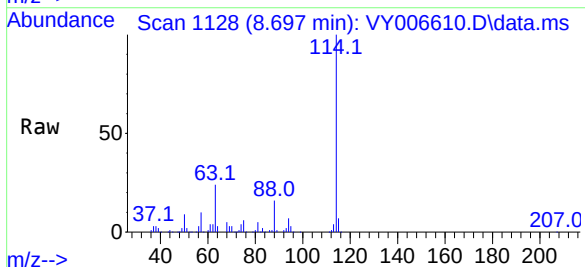


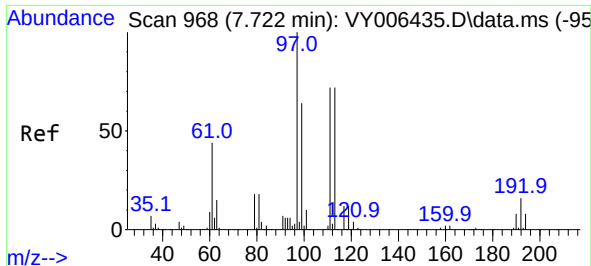

#35
Dibromofluoromethane
Concen: 56.430 ug/l
RT: 7.728 min Scan# 968
Delta R.T. 0.006 min
Lab File: VY006610.D
Acq: 03 Nov 2021 18:41




Instrument :
MSVOA_Y
ClientSampleId :
WC-2-KD


Tgt Ion:113 Resp: 37899
Ion Ratio Lower Upper
113 100
111 101.6 82.3 123.5
192 20.3 17.4 26.2

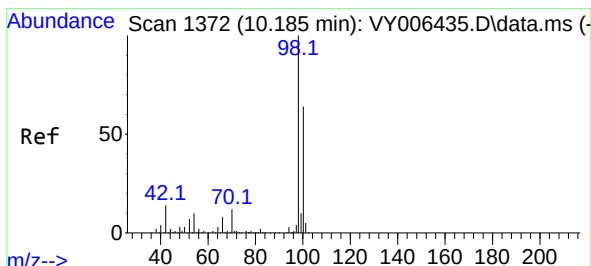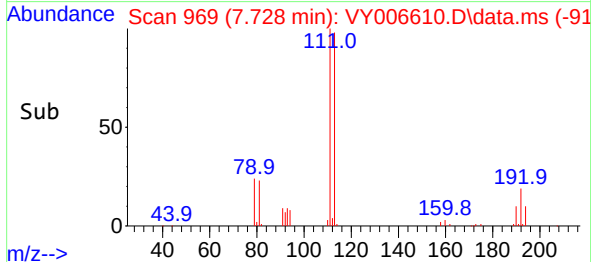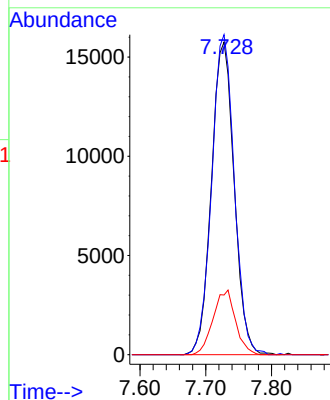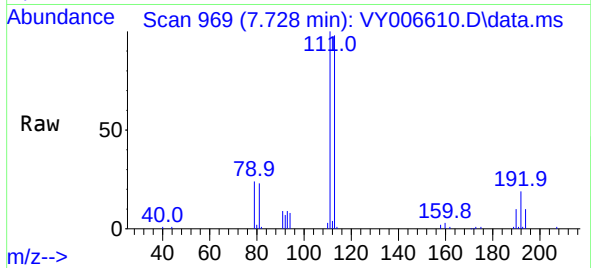

#50
Toluene-d8
Concen: 53.632 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY006610.D
Acq: 03 Nov 2021 18:41

Tgt Ion: 98 Resp: 152693
Ion Ratio Lower Upper
98 100
100 63.0 50.9 76.3


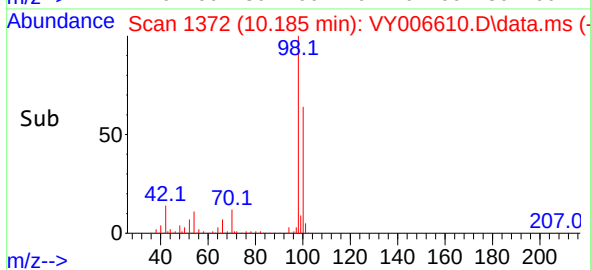
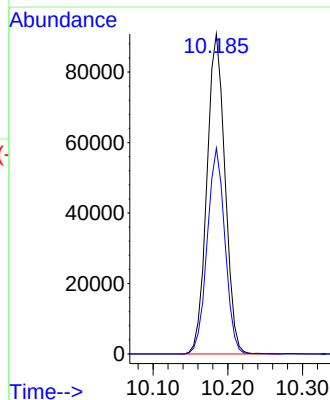
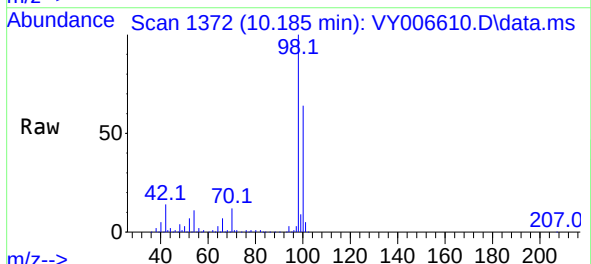


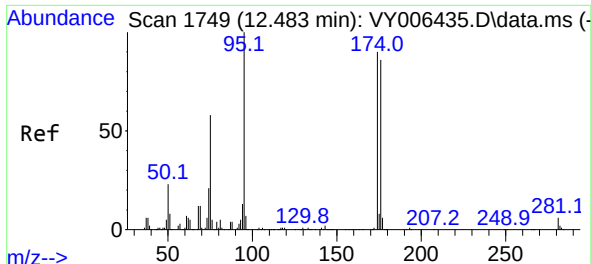

#62
4-Bromofluorobenzene
Concen: 46.974 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY006610.D
Acq: 03 Nov 2021 18:41




Instrument :
MSVOA_Y
ClientSampleId :
WC-2-KD


Tgt Ion: 95 Resp: 45051
Ion Ratio Lower Upper
95 100
174 83.3 0.0 177.0
176 80.2 0.0 169.4

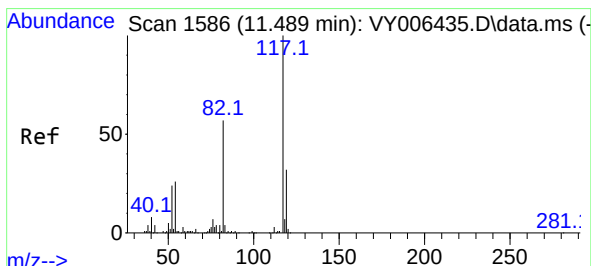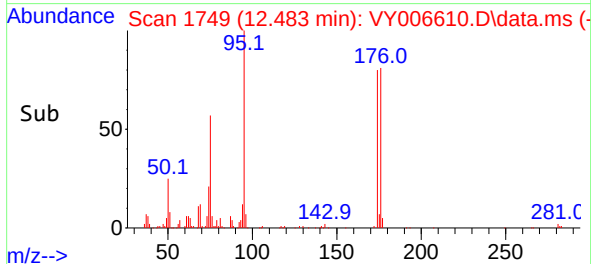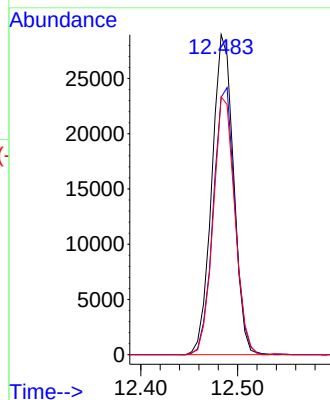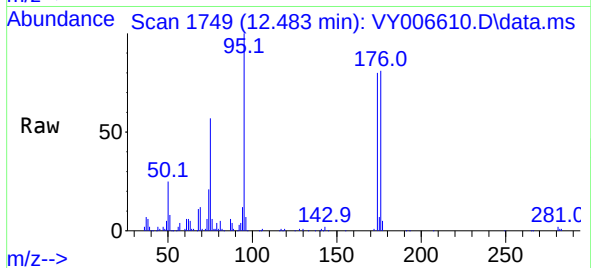

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.495 min Scan# 1587
Delta R.T. 0.006 min
Lab File: VY006610.D
Acq: 03 Nov 2021 18:41

Tgt Ion: 117 Resp: 108434
Ion Ratio Lower Upper
117 100
82 59.6 45.7 68.5
119 31.7 25.5 38.3

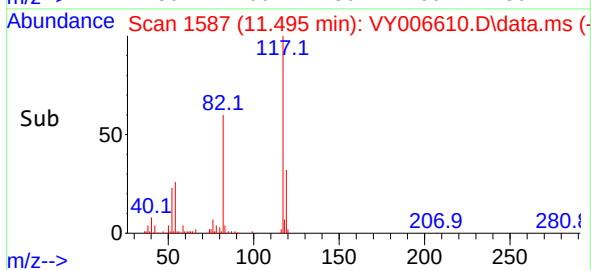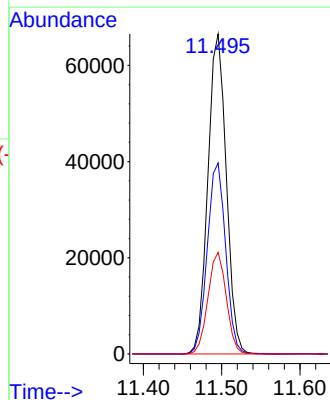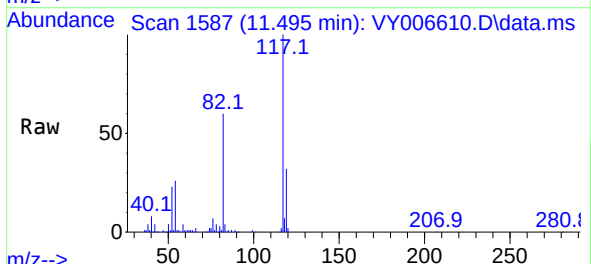

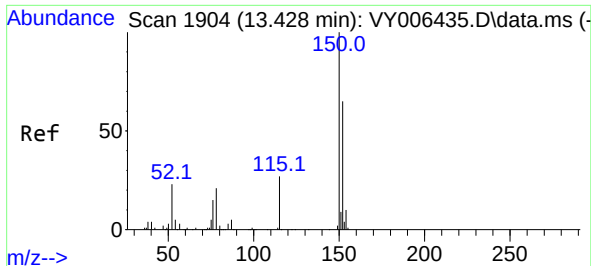

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.428 min Scan# 1904
 Delta R.T. -0.000 min
 Lab File: VY006610.D
 Acq: 03 Nov 2021 18:41

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-2-KD

Tgt Ion:152 Resp: 40363
 Ion Ratio Lower Upper
 152 100
 115 60.3 28.5 85.5
 150 162.1 0.0 348.2

