
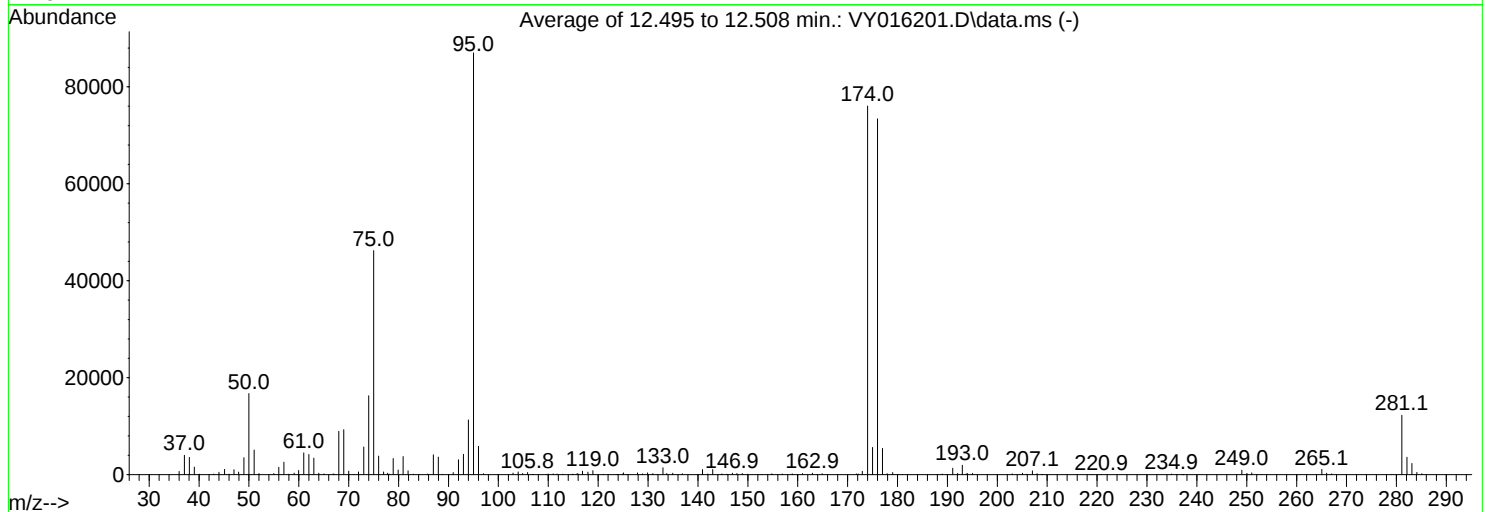


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110323\
Data File : VY016201.D
Acq On : 03 Nov 2023 08:19
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103123S.M
Title : SW846 8260
Last Update : Wed Nov 01 03:33:29 2023

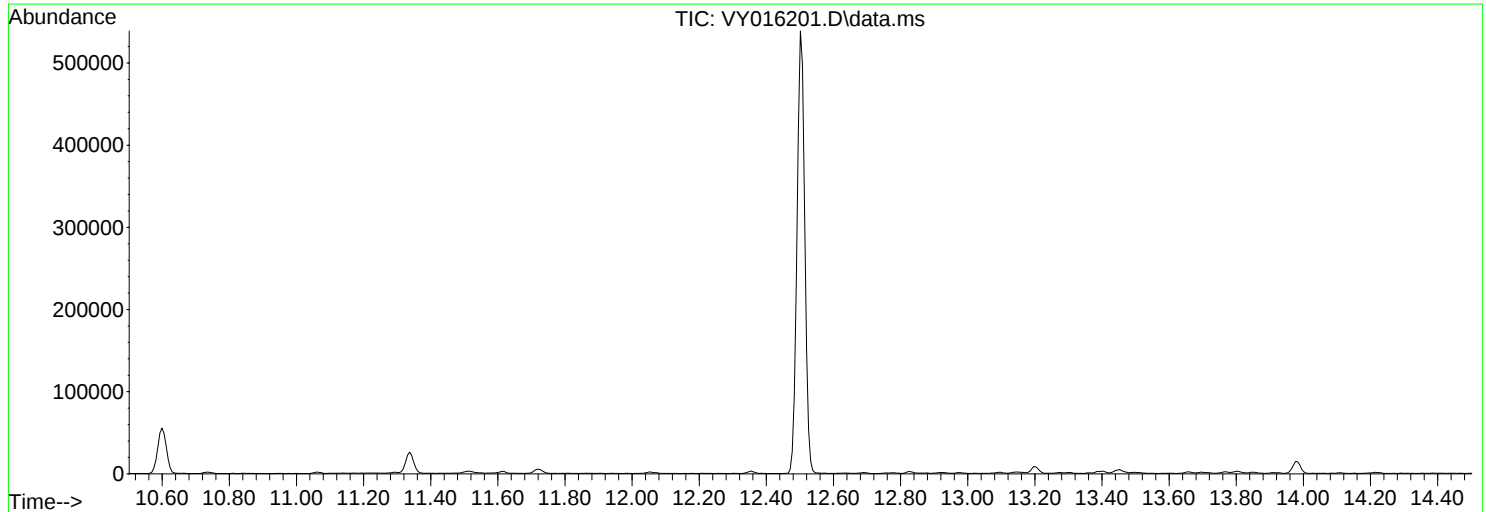

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1742

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	16720	PASS
75	95	30	60	53.1	46221	PASS
95	95	100	100	100.0	87011	PASS
96	95	5	9	6.7	5845	PASS
173	174	0.00	2	0.9	691	PASS
174	95	50	100	87.4	76037	PASS
175	174	5	9	7.4	5621	PASS
176	174	95	101	96.5	73403	PASS
177	176	5	9	7.4	5408	PASS