


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110323\
Data File : VY016216.D
Acq On : 03 Nov 2023 16:31
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103123S.M
Title : SW846 8260
Last Update : Wed Nov 01 03:33:29 2023

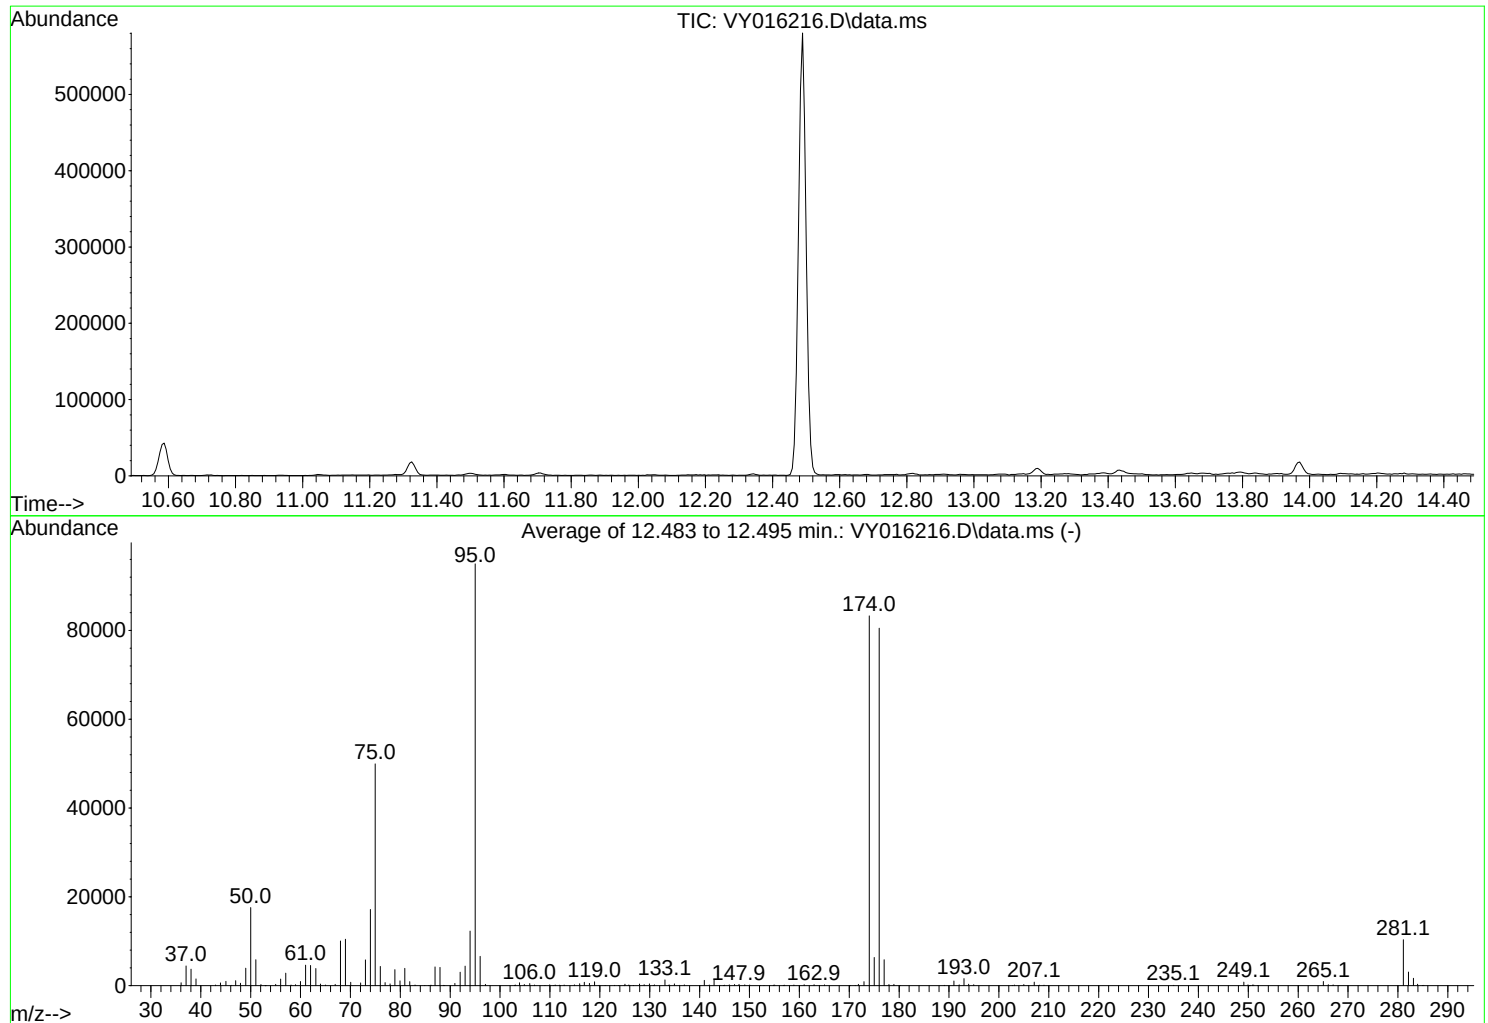

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	17579	PASS
75	95	30	60	52.6	49946	PASS
95	95	100	100	100.0	94984	PASS
96	95	5	9	7.0	6602	PASS
173	174	0.00	2	1.1	900	PASS
174	95	50	100	87.7	83285	PASS
175	174	5	9	7.6	6354	PASS
176	174	95	101	96.6	80477	PASS
177	176	5	9	7.2	5827	PASS