

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY110519\
 Data File : VY000537.D
 Acq On : 05 Nov 2019 15:22
 Operator : SY/MD
 Sample : K5202-05
 Misc : 5.26G/10ML/MSVOA Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 C0AA9

Quant Time: Nov 06 07:04:24 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SFAMYL110519SMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 06 07:01:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.70	114	354258	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.49	117	312358	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.42	152	133894	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.24	65	138532	25.67	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.68%
7) Chloroethane-d5	2.77	69	120775	25.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.76%
11) 1,1-Dichloroethene-d2	3.86	63	177518	18.95	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.80%
21) 2-Butanone-d5	6.91	46	81913	34.57	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	69.14%
24) Chloroform-d	7.49	84	220613	23.89	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.56%
26) 1,2-Dichloroethane-d4	8.16	65	131884	23.66	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.64%
32) Benzene-d6	8.12	84	473128	26.19	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	104.76%
36) 1,2-Dichloropropane-d6	9.13	67	143672	26.10	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.40%
41) Toluene-d8	10.18	98	426472	25.40	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	101.60%
43) trans-1,3-Dichloropropene-	10.44	79	64673	23.28	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.12%
47) 2-Hexanone-d5	10.79	63	64747	37.58	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.16%
56) 1,1,2,2-Tetrachloroethane-	12.56	84	120936	20.29	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.16%
66) 1,2-Dichlorobenzene-d4	13.72	152	126317	24.15	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.60%

Target Compounds


					Ovalue
13) Acetone	3.98	43	11692	5.172	ug/L 86
16) Methylene chloride	4.72	84	5286	0.916	ug/L 88
44) trans-1,3-Dichloropropene	10.44	75	3554	0.480	ug/L 98
60) Isopropylbenzene	12.33	105	1545	0.072	ug/L # 87
61) 1,2,3-Trichloropropane	12.64	75	245	0.058	ug/L # 35
62) 1,3,5-Trimethylbenzene	12.33	105	1545	0.088	ug/L 93
63) 1,2,4-Trimethylbenzene	13.12	105	2420	0.141	ug/L 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY110519\
Data File : VY000537.D
Acq On : 05 Nov 2019 15:22
Operator : SY/MD
Sample : K5202-05
Misc : 5.26G/10ML/MSVOA Y/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
C0AA9

Quant Time: Nov 06 07:04:24 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\SFAMYL110519SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 06 07:01:34 2019
Response via : Initial Calibration

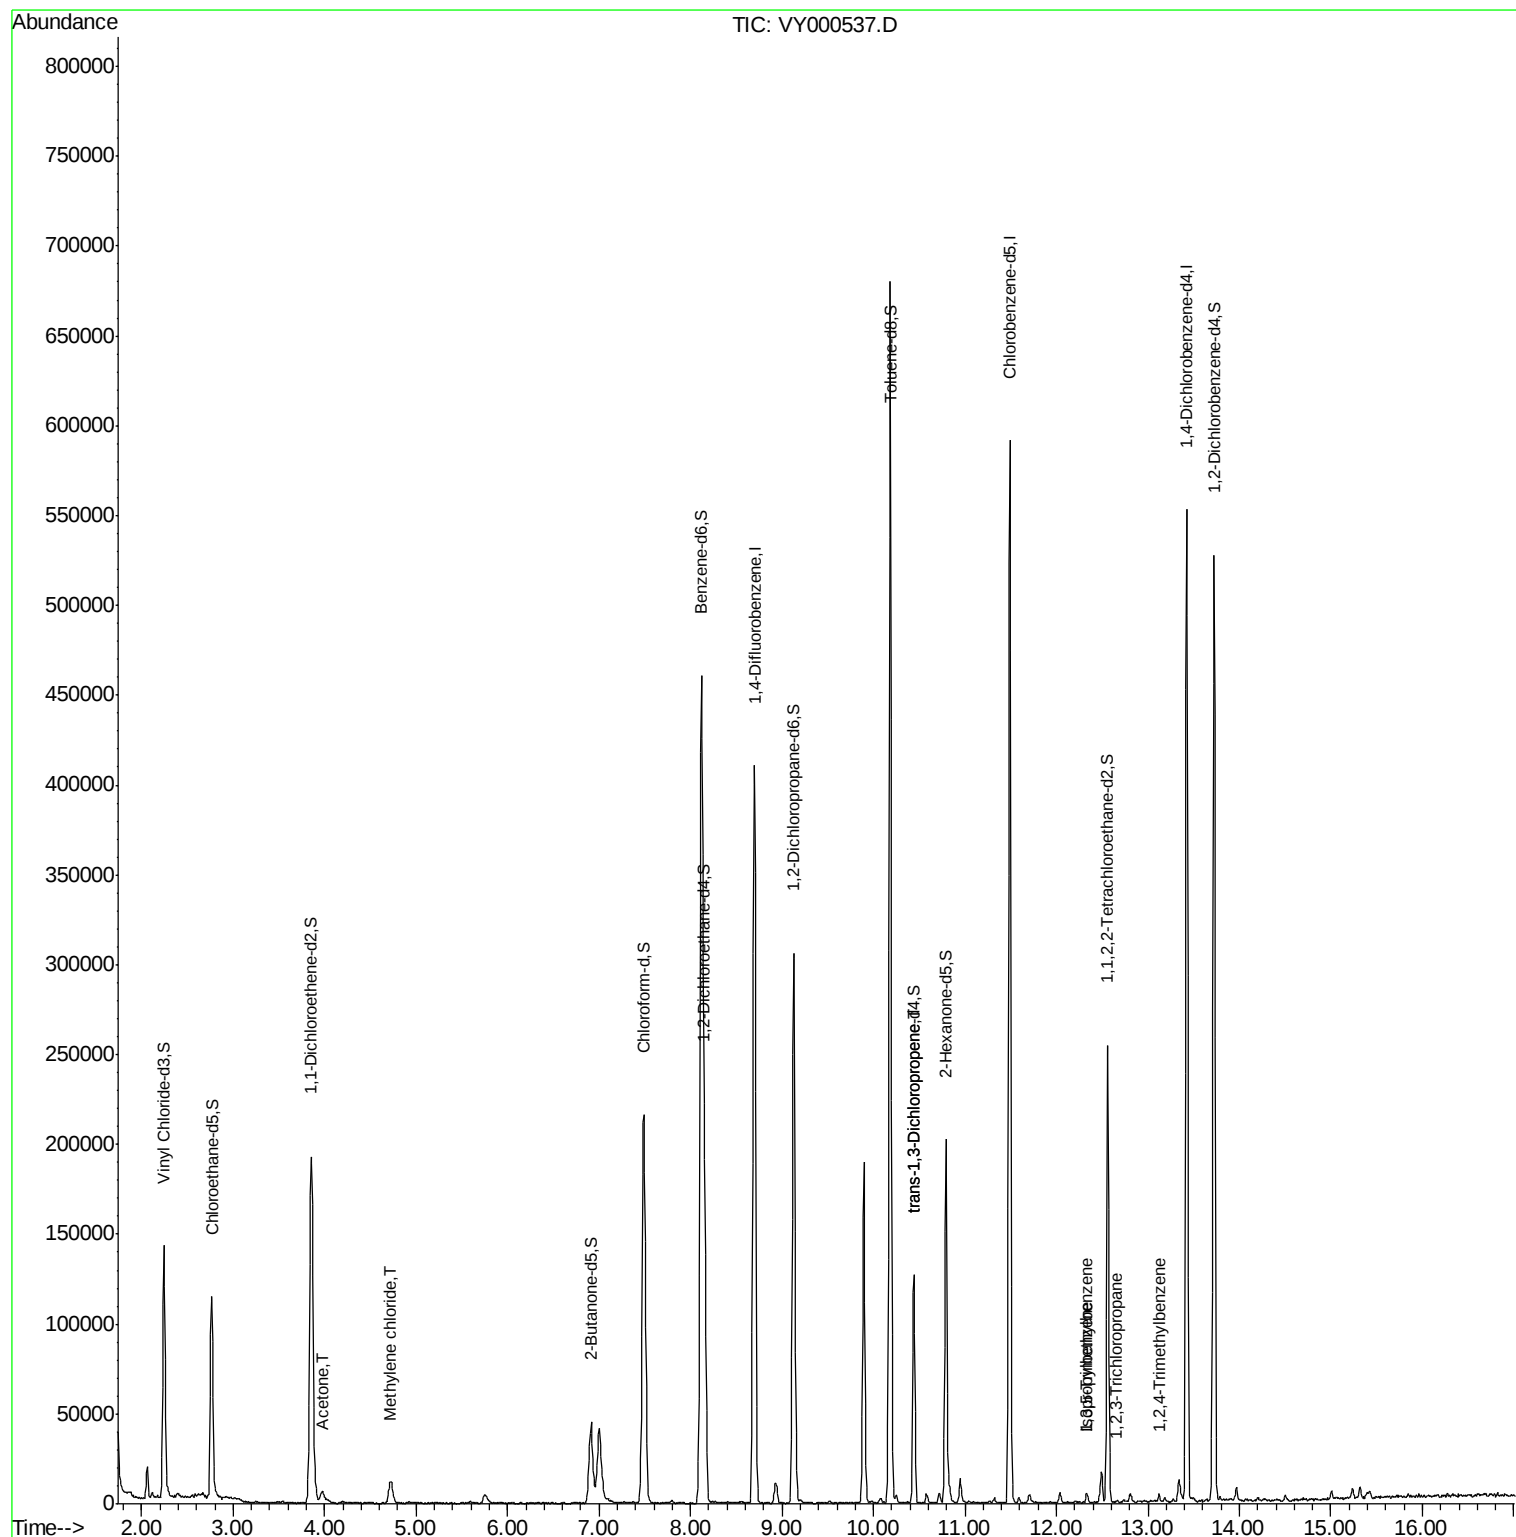

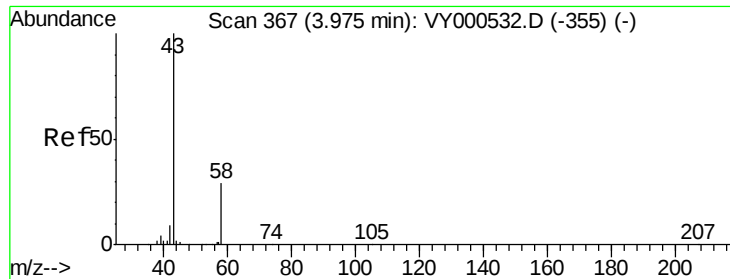

#13

Acetone

Concen: 5.172 ug/L

RT: 3.98 min Scan# 368

Delta R.T. 0.01 min

Lab File: VY000537.D

Acq: 05 Nov 2019 15:22

Instrument :

MSVOA_Y

ClientSampleId :


C0AA9

Tot Ion: 43 Resp: 11692

Ion Ratio Lower Upper




43 100

58 26.7 0.0 69.6

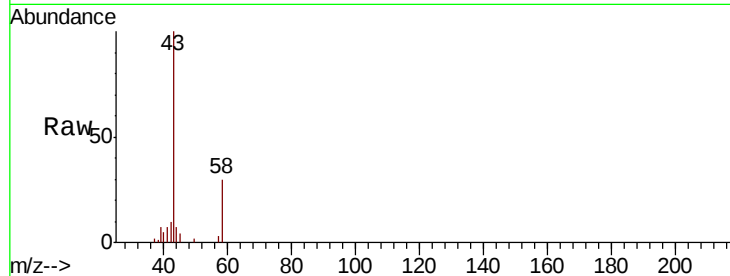

Abundance Ion 43.00 (42.70 to 43.70): VY000532.D (-355) (-)

Ion 58.00 (57.70 to 58.70): VY000532.D (-355) (-)

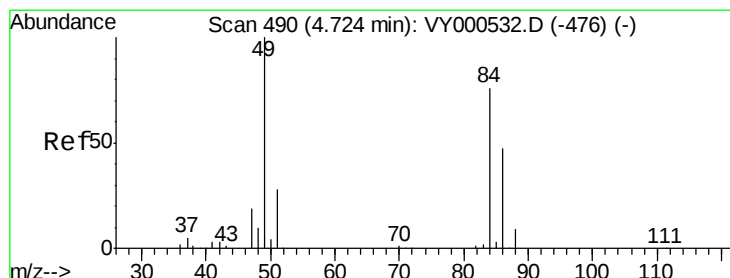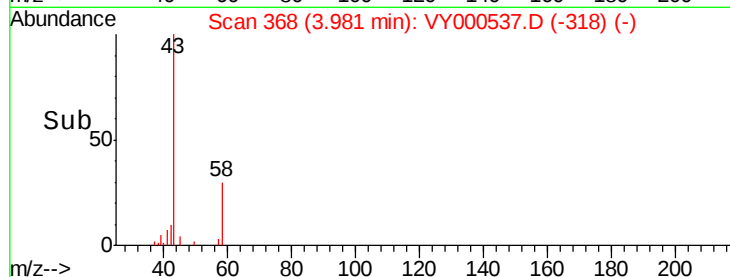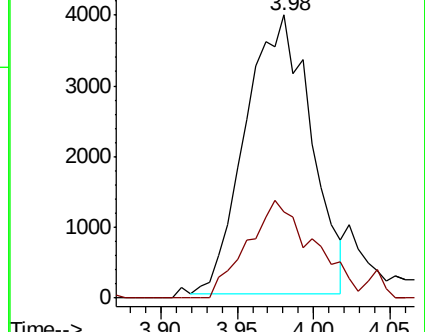

#16

Methylene chloride

Concen: 0.916 ug/L

RT: 4.72 min Scan# 489

Delta R.T. -0.01 min

Lab File: VY000537.D

Acq: 05 Nov 2019 15:22


Tgt Ion: 84 Resp: 5286

Ion Ratio Lower Upper

84 100

86 61.9 43.4 80.6



49 111.9 92.3 171.3

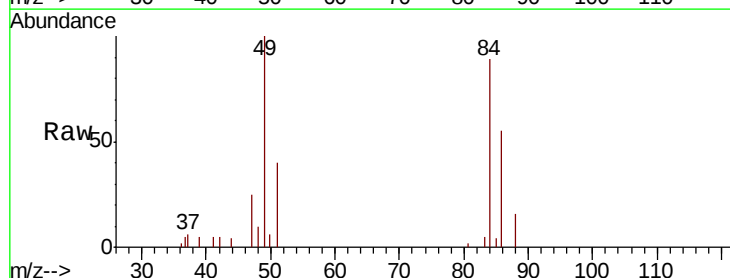


Abundance Ion 84.00 (83.70 to 84.70): VY000532.D (-476) (-)

Ion 86.00 (85.70 to 86.70): VY000532.D (-476) (-)

Ion 49.00 (48.70 to 49.70): VY000532.D (-476) (-)

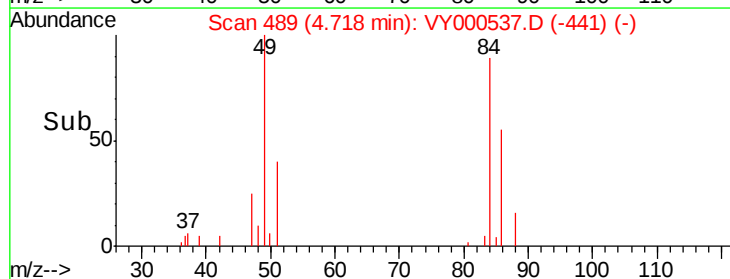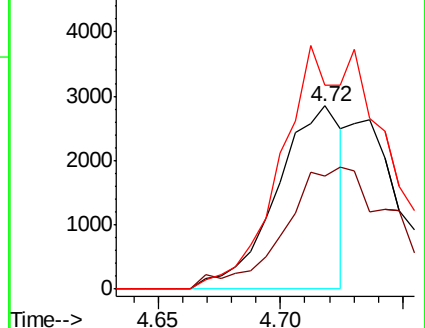

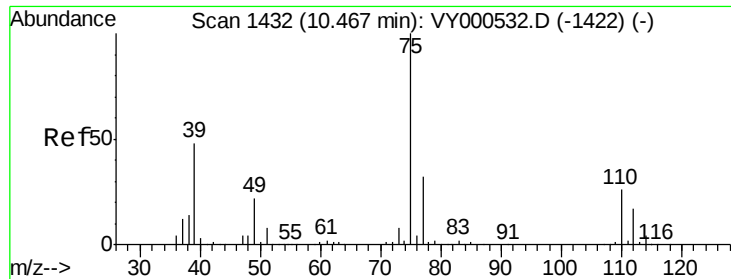

#44

trans-1,3-Dichloropropene

Concen: 0.480 ug/L

RT: 10.44 min Scan# 1427

Delta R.T. -0.03 min

Lab File: VY000537.D

Acq: 05 Nov 2019 15:22

Instrument :

MSVOA_Y

ClientSampled :


C0AA9

Tot Ion: 75 Resp: 3554

Ion Ratio Lower Upper

75 100

77 31.3 22.7 42.1

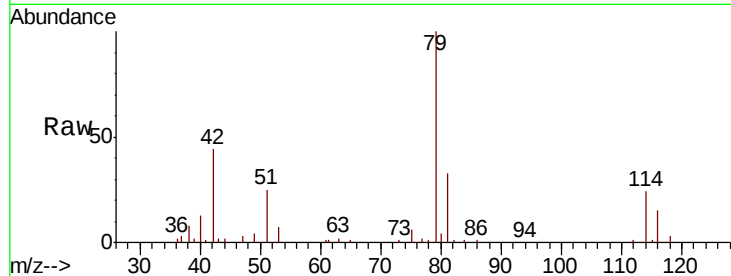

Abundance Ion 75.00 (74.70 to 75.70): VY000532.D (-1422) (-)

Ion 77.00 (76.70 to 77.70): VY000532.D (-1422) (-)

10.44

2000

1500

1000

500



0

10.40

10.45

10.50

Time-->

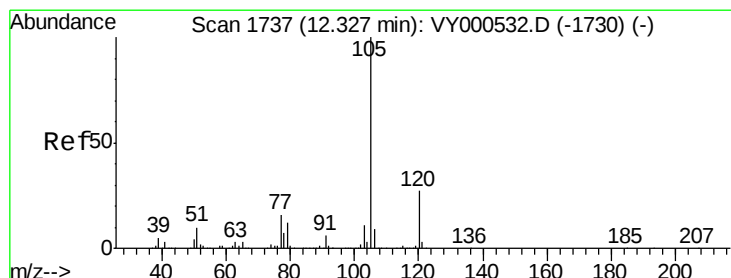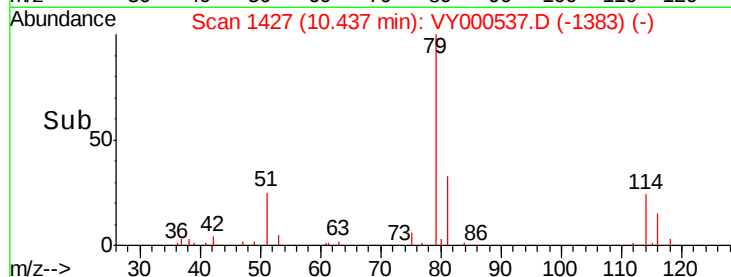

#60

Isopropylbenzene

Concen: 0.072 ug/L

RT: 12.33 min Scan# 1737

Delta R.T. -0.00 min

Lab File: VY000537.D

Acq: 05 Nov 2019 15:22


Tgt Ion: 105 Resp: 1545

Ion Ratio Lower Upper

105 100

120 28.7 21.8 32.8

77 28.7 12.6 19.0#

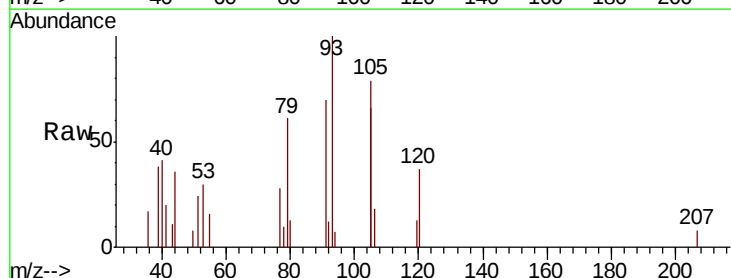

Abundance Ion 105.00 (104.70 to 105.70): VY000532.D (-1730) (-)

Ion 120.00 (119.70 to 120.70): VY000532.D (-1730) (-)

Ion 77.00 (76.70 to 77.70): VY000532.D (-1730) (-)

12.33

1500

1000


500


0

12.30

12.35

Time-->

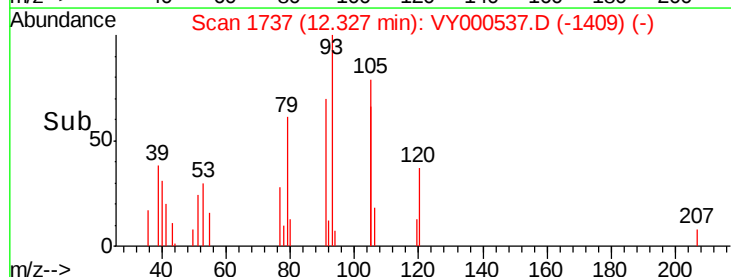

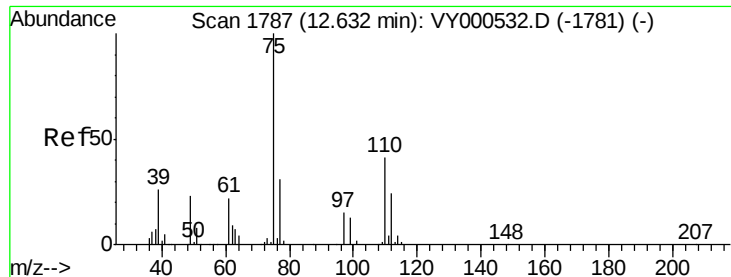

#61

1,2,3-Trichloropropane

Concen: 0.058 ug/L

RT: 12.64 min Scan# 1789

Delta R.T. 0.01 min

Lab File: VY000537.D

Acq: 05 Nov 2019 15:22

Instrument :

MSVOA_Y

ClientSampled :

C0AA9





Tot Ion: 75 Resp: 245

Ion Ratio Lower Upper

75 100

77 67.3 25.4 38.0#

110 0.0 33.0 49.4#

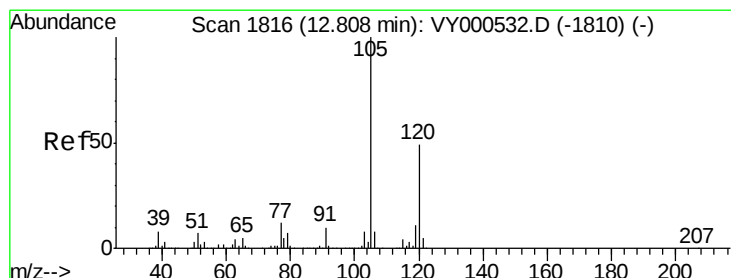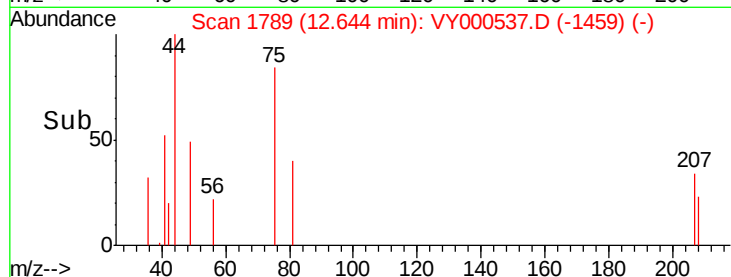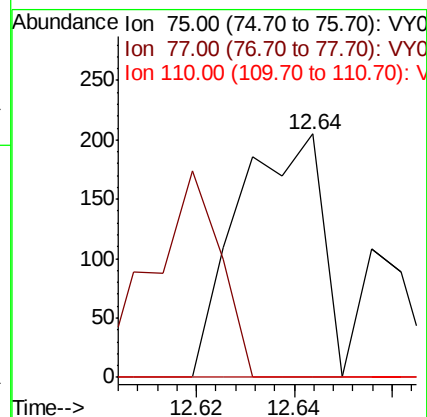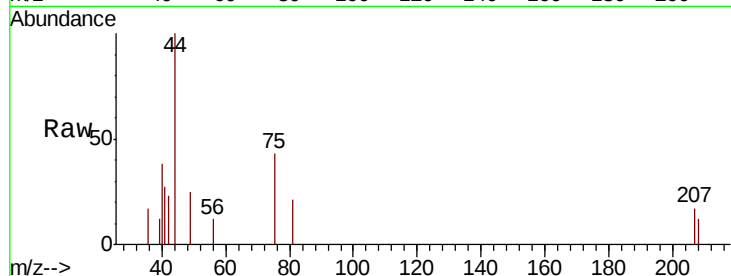

#62

1,3,5-Trimethylbenzene

Concen: 0.088 ug/L

RT: 12.33 min Scan# 1737

Delta R.T. -0.48 min

Lab File: VY000537.D




Acq: 05 Nov 2019 15:22


Tgt Ion: 105 Resp: 1545

Ion Ratio Lower Upper

105 100

120 28.7 25.9 38.9

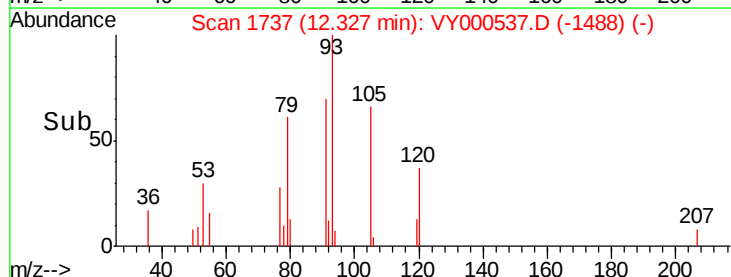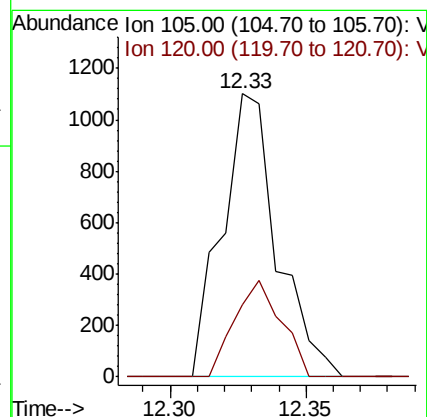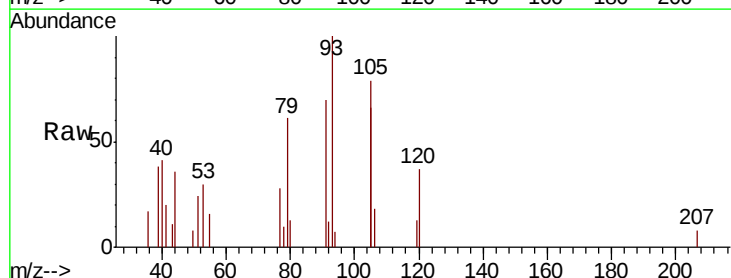

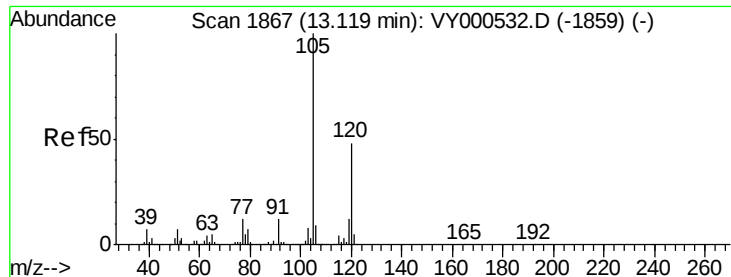

#63

1,2,4-Trimethylbenzene

Concen: 0.141 ug/L

RT: 13.12 min Scan# 1867

Delta R.T. -0.00 min

Lab File: VY000537.D

Acq: 05 Nov 2019 15:22

Instrument :

MSVOA_Y

ClientSampleId :


C0AA9

Tot Ion:105 Resp: 2420

Ion Ratio Lower Upper

105 100

120 48.3 40.3 60.5

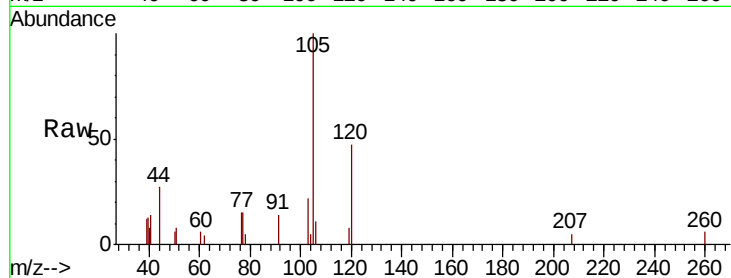

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

