


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv110520\
 Data File : VY003515.D
 Acq On : 05 Nov 2020 09:16
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y110220S.M
 Title : SW846 8260
 Last Update : Mon Nov 02 12:40:51 2020

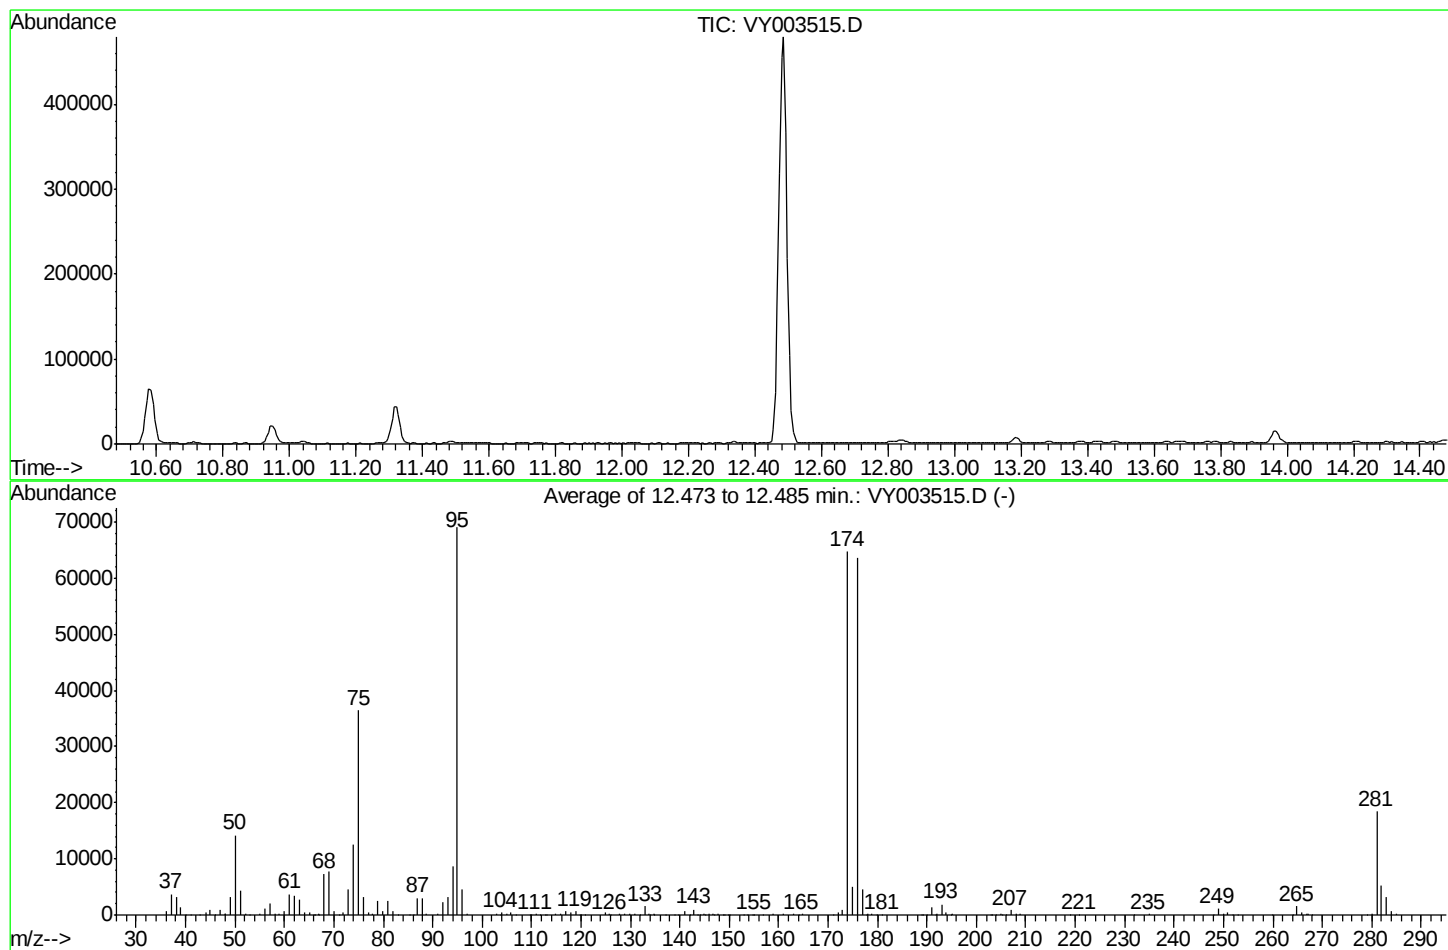

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	14152	PASS
75	95	30	60	52.8	36421	PASS
95	95	100	100	100.0	69032	PASS
96	95	5	9	6.6	4568	PASS
173	174	0.00	2	1.5	998	PASS
174	95	50	100	93.7	64698	PASS
175	174	5	9	7.8	5059	PASS
176	174	95	101	98.3	63621	PASS
177	176	5	9	7.2	4551	PASS