
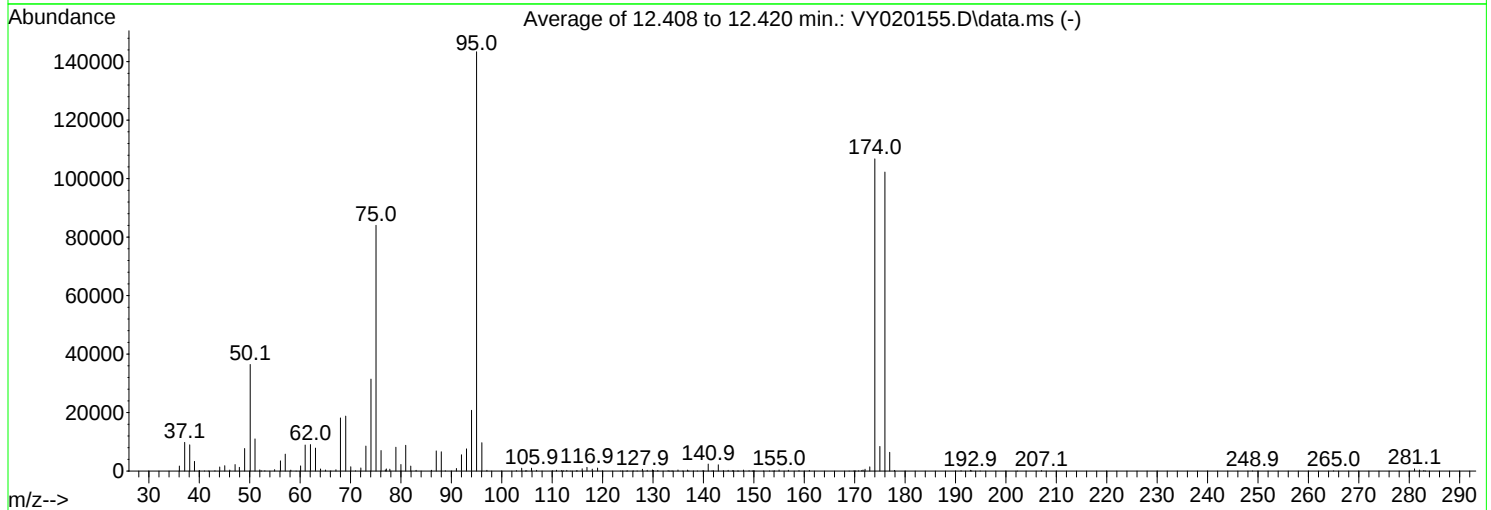


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110524\
Data File : VY020155.D
Acq On : 05 Nov 2024 08:32
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103024S.M
Title : SW846 8260
Last Update : Thu Oct 31 15:23:13 2024

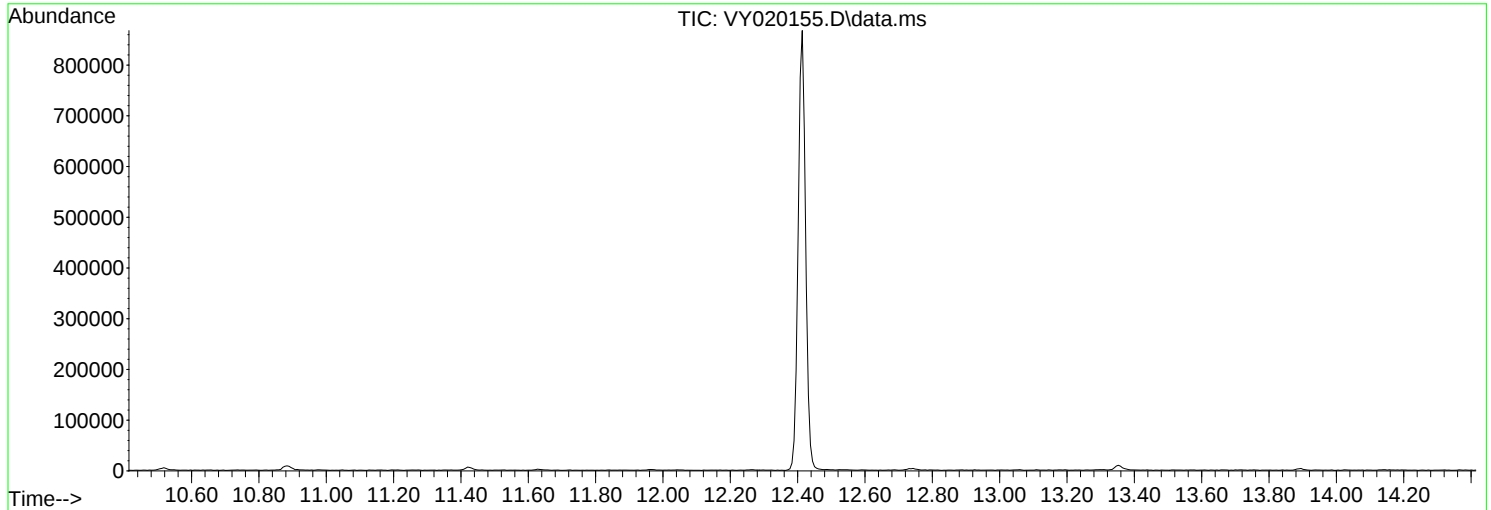

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.4	36459	PASS
75	95	30	60	58.6	84035	PASS
95	95	100	100	100.0	143384	PASS
96	95	5	9	6.8	9710	PASS
173	174	0.00	2	1.4	1450	PASS
174	95	50	100	74.5	106757	PASS
175	174	5	9	7.9	8419	PASS
176	174	95	101	95.8	102240	PASS
177	176	5	9	6.3	6426	PASS