

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_Y\DATA\VY110619\
 Data File : VY000562.D
 Acq On : 06 Nov 2019 19:14
 Operator : SY/MD
 Sample : K5723-03
 Misc : 7.32G/5ML/MSVOA_Y/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 7-C

Quant Time: Nov 07 06:22:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 30 13:30:53 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	231141	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.70	114	421422	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	368389	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	150976	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.15	65	139587	58.36	ug/l	0.00
Spiked Amount 50.000			Recovery	=	116.72%	
35) Dibromofluoromethane	7.73	113	124717	50.41	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.82%	
50) Toluene-d8	10.18	98	503593	53.64	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.28%	
62) 4-Bromofluorobenzene	12.48	95	159997	44.77	ug/l	0.00
Spiked Amount 50.000			Recovery	=	89.54%	
Target Compounds						
20) Methylene Chloride	4.73	84	19831	7.020	ug/l	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_Y\DATA\VY110619\
Data File : VY000562.D
Acq On : 06 Nov 2019 19:14
Operator : SY/MD
Sample : K5723-03
Misc : 7.32G/5ML/MSVOA_Y/SOIL
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
7-C

Quant Time: Nov 07 06:22:43 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 30 13:30:53 2019
Response via : Initial Calibration

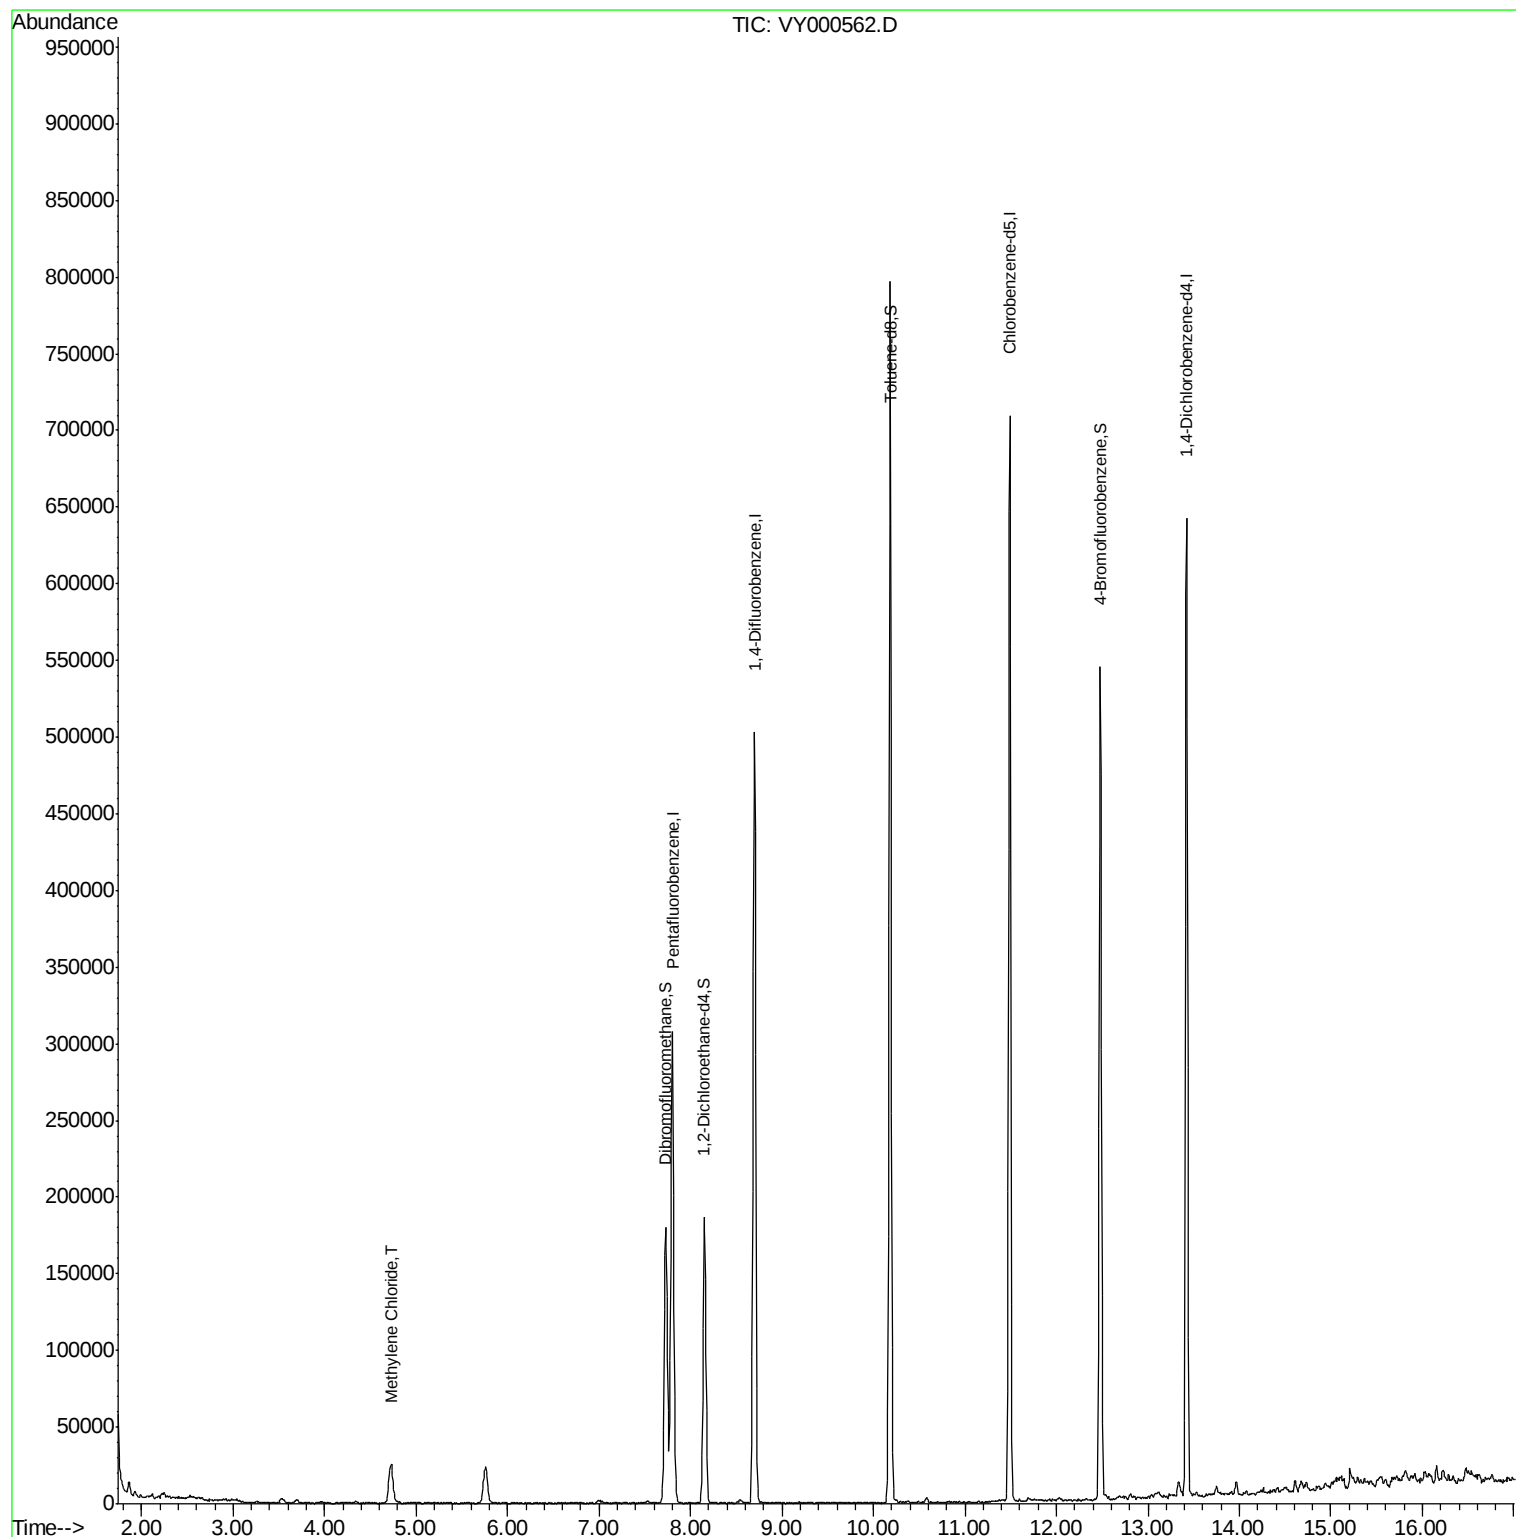

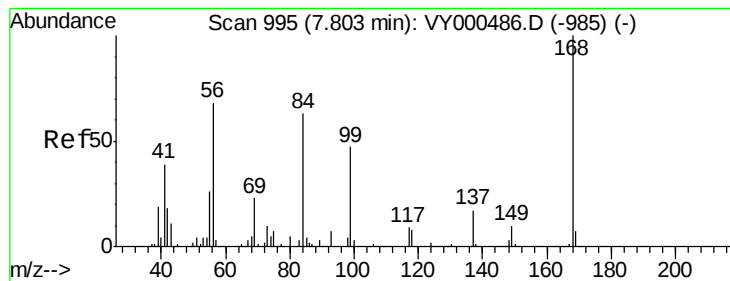

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 995

Delta R.T. 0.00 min

Lab File: VY000562.D

Acq: 06 Nov 2019 19:14


Instrument :
MSVOA_Y
ClientSampleId :
7-C

Tgt Ion: 168 Resp: 231141

Ion Ratio Lower Upper

168 100

99 55.3 45.7 68.5

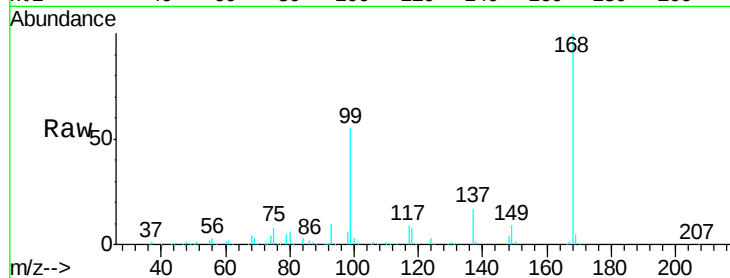

Abundance Ion 167.90 (167.60 to 168.60): VY000486.D (-985) (-)

Ion 98.90 (98.60 to 99.60): VY000486.D (-985) (-)

7.80

120000

100000

80000



60000

40000

20000

0

Time-->

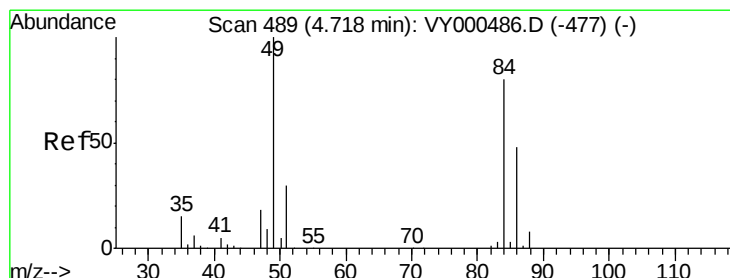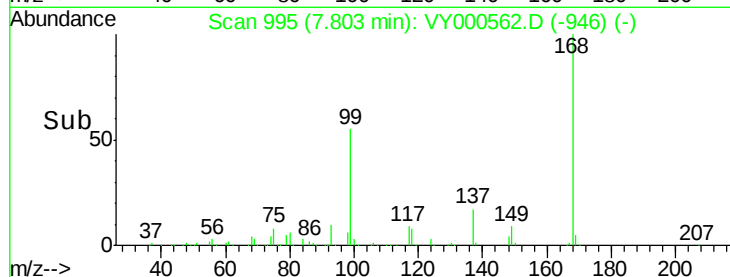

#20

Methylene Chloride

Concen: 7.020 ug/l

RT: 4.73 min Scan# 491

Delta R.T. 0.01 min

Lab File: VY000562.D

Acq: 06 Nov 2019 19:14

Tgt Ion: 84 Resp: 19831


Ion Ratio Lower Upper

84 100

49 104.3 100.2 150.4

51 36.8 29.6 44.4

86 62.0 48.3 72.5

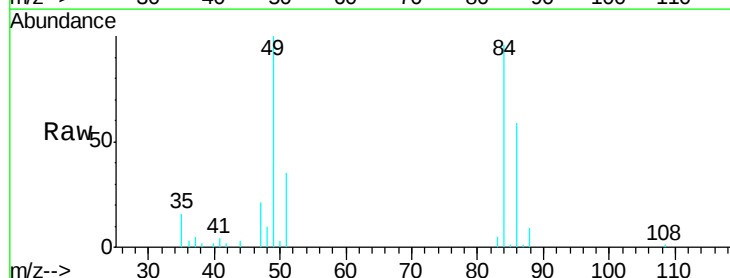

Abundance Ion 83.90 (83.60 to 84.60): VY000486.D (-477) (-)

Ion 48.90 (48.60 to 49.60): VY000486.D (-477) (-)

Ion 50.90 (50.60 to 51.60): VY000486.D (-477) (-)

Ion 85.90 (85.60 to 86.60): VY000486.D (-477) (-)

4.73

12000

10000

8000


6000


4000

2000

0

Time-->




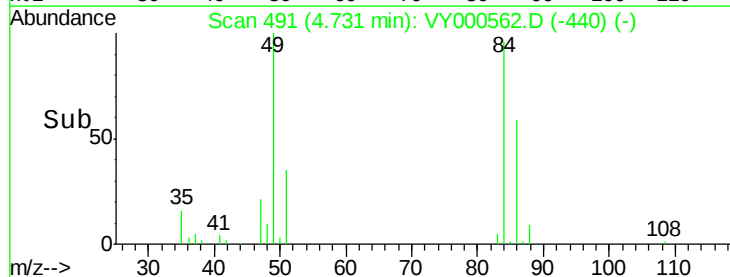


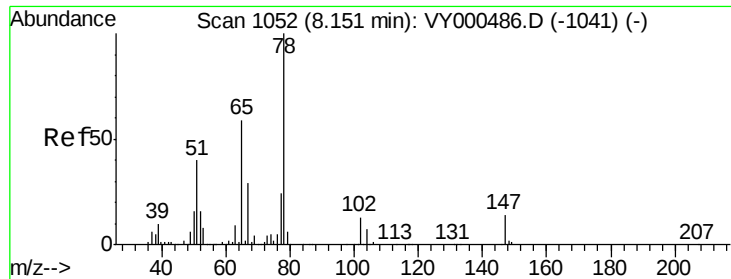

#33
 1,2-Dichloroethane-d4
 Concen: 58.356 ug/l
 RT: 8.15 min Scan# 1052
 Delta R.T. 0.00 min
 Lab File: VY000562.D
 Acq: 06 Nov 2019 19:14




Instrument :
 MSVOA_Y
 ClientSampleId :
 7-C


Tgt Ion: 65 Resp: 139587
 Ion Ratio Lower Upper
 65 100
 67 53.4 0.0 107.2

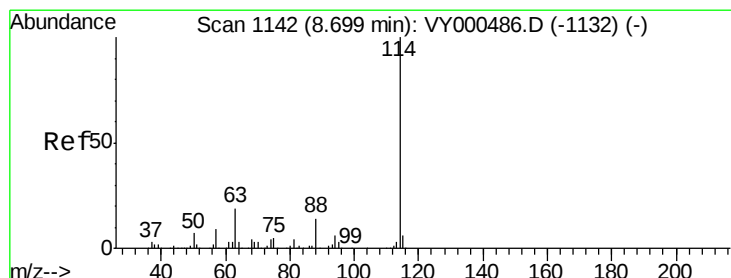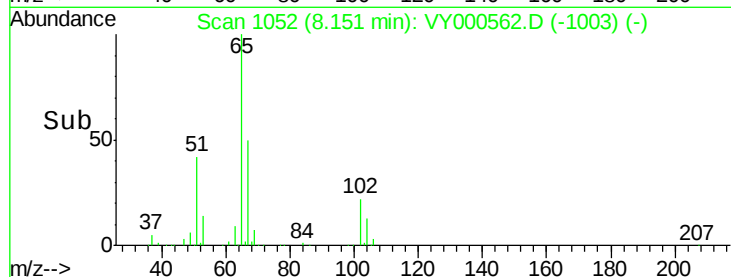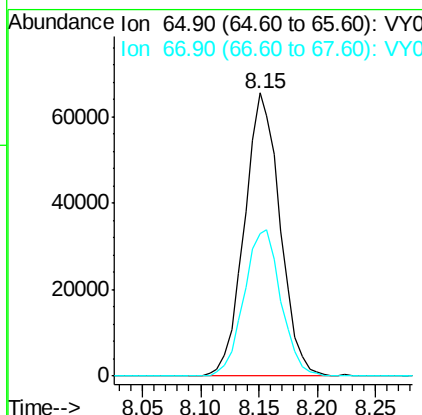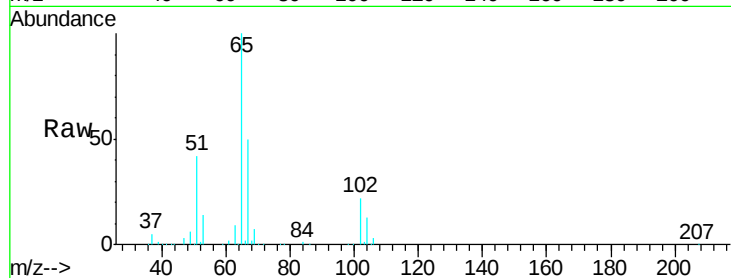

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.70 min Scan# 1142
 Delta R.T. 0.00 min
 Lab File: VY000562.D
 Acq: 06 Nov 2019 19:14

Tgt Ion: 114 Resp: 421422
 Ion Ratio Lower Upper
 114 100
 63 20.4 0.0 38.0
 88 15.1 0.0 28.6


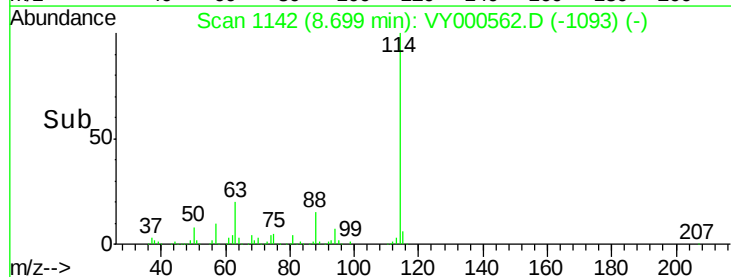
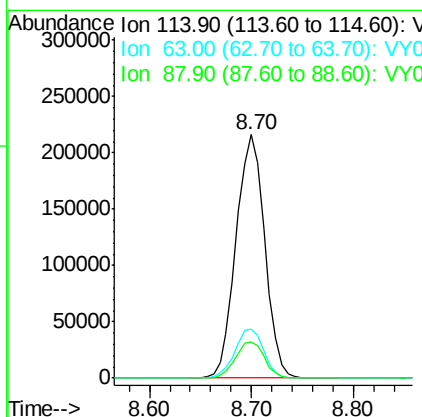
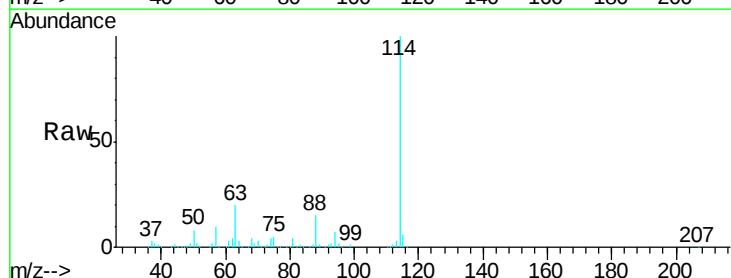


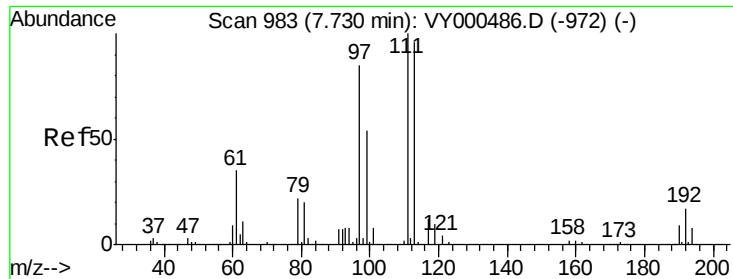

#35
 Dibromofluoromethane
 Concen: 50.411 ug/l
 RT: 7.73 min Scan# 983
 Delta R.T. 0.00 min
 Lab File: VY000562.D
 Acq: 06 Nov 2019 19:14




Instrument :
 MSVOA_Y
 ClientSampled :
 7-C


Tgt Ion:113 Resp: 124717
 Ion Ratio Lower Upper
 113 100
 111 101.5 81.7 122.5
 192 18.9 15.0 22.4

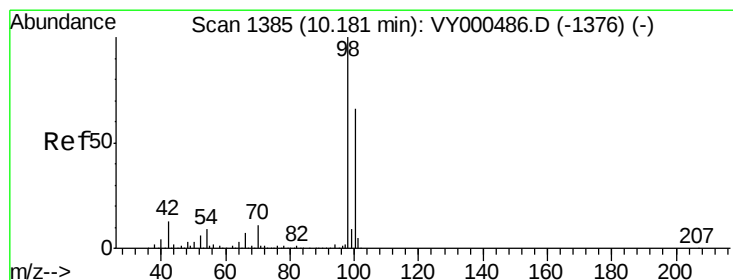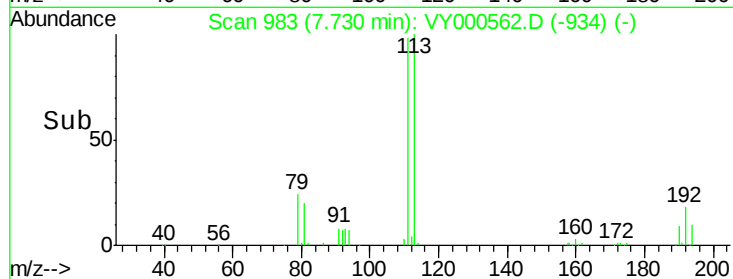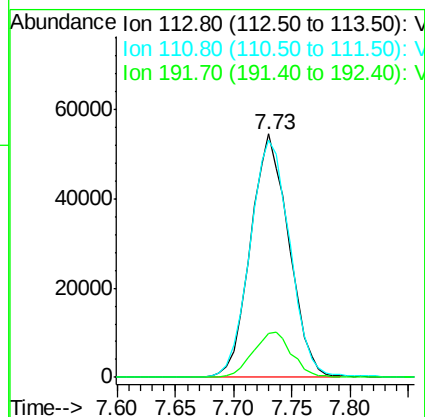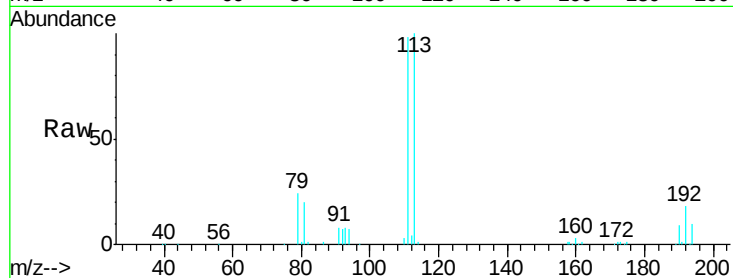

#50
 Toluene-d8
 Concen: 53.645 ug/l
 RT: 10.18 min Scan# 1385
 Delta R.T. 0.00 min
 Lab File: VY000562.D
 Acq: 06 Nov 2019 19:14

Tgt Ion: 98 Resp: 503593
 Ion Ratio Lower Upper
 98 100
 100 64.5 52.9 79.3


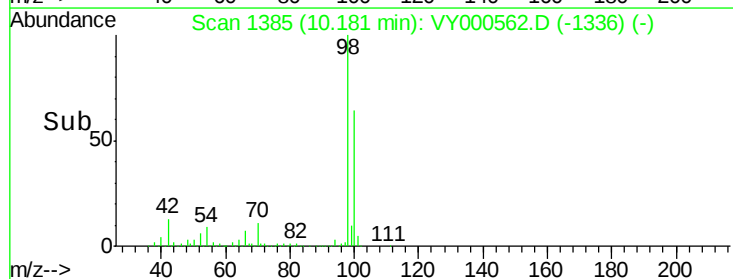
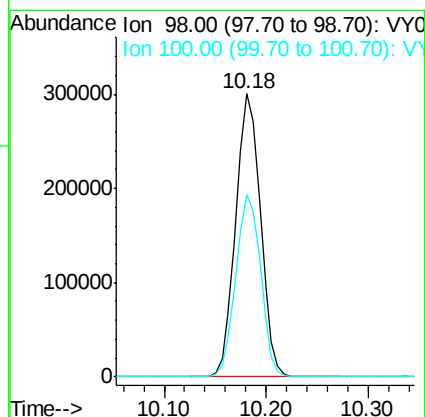
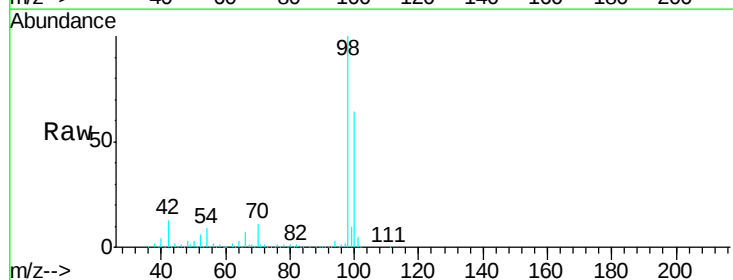


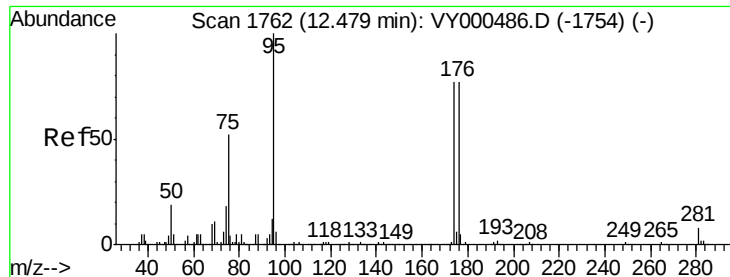

#62
4-Bromofluorobenzene
Concen: 44.769 ug/l
RT: 12.48 min Scan# 1762
Delta R.T. 0.00 min
Lab File: VY000562.D
Acq: 06 Nov 2019 19:14




Instrument :
MSVOA_Y
ClientSampled :
7-C


Tgt Ion	Ratio	Lower	Upper
95	100		
174	79.2	0.0	161.6
176	75.3	0.0	157.8

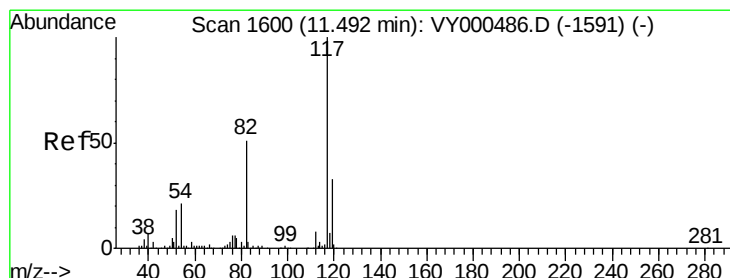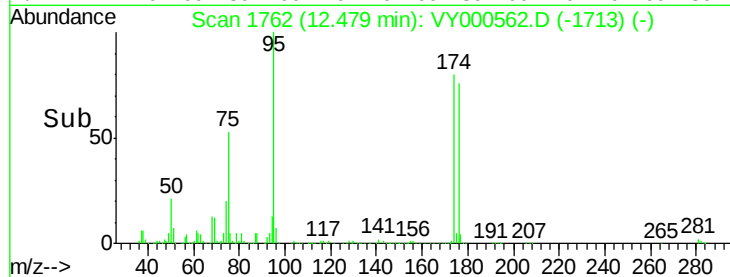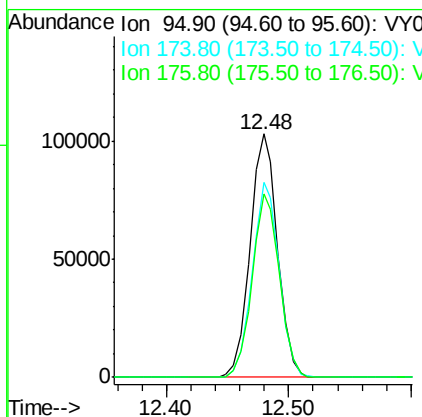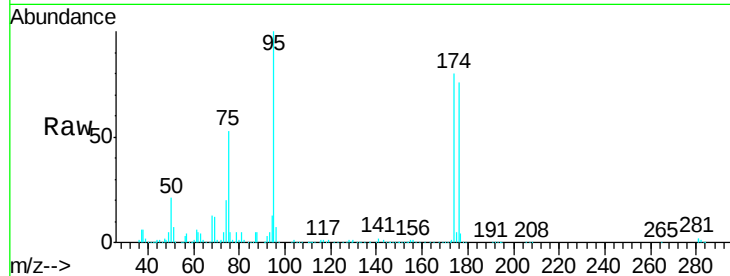

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. 0.00 min
Lab File: VY000562.D
Acq: 06 Nov 2019 19:14

Tgt Ion	Ratio	Lower	Upper
117	100		
82	57.0	40.8	61.2
119	32.5	26.2	39.2

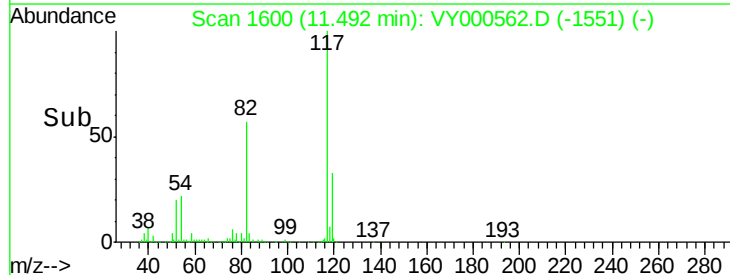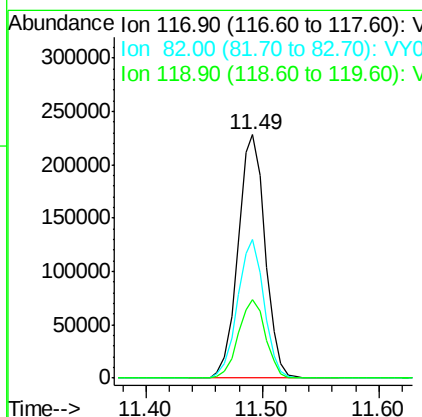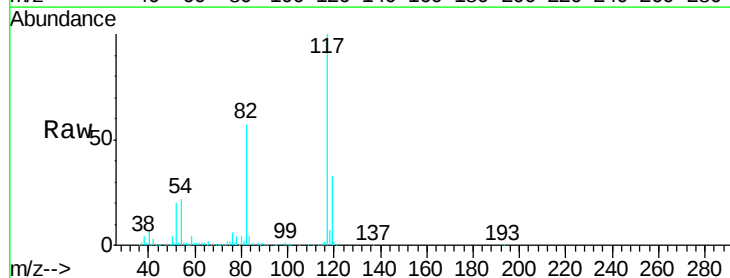

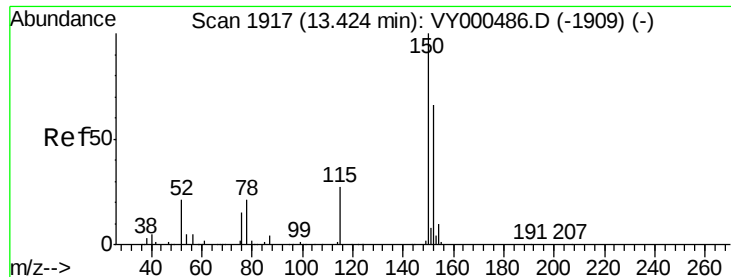


#72

1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.42 min Scan# 1917
 Delta R.T. 0.00 min
 Lab File: VY000562.D
 Acq: 06 Nov 2019 19:14

Instrument :
 MSVOA_Y
 ClientSampleId :
 7-C

Tgt Ion	Ratio	Lower	Upper
152	100		
115	62.3	29.1	87.4
150	162.9	0.0	348.8

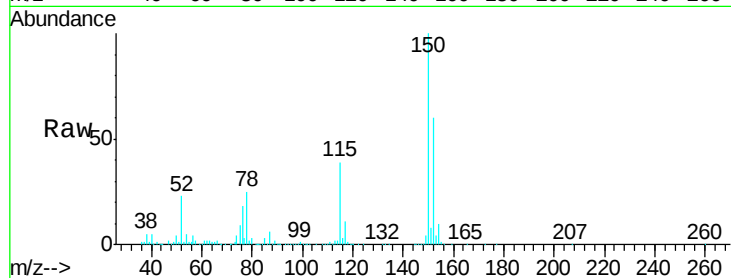

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

