


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\vy110619\
 Data File : VY000539.D
 Acq On : 06 Nov 2019 09:29
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
 Title : SW846 8260
 Last Update : Wed Oct 30 13:30:53 2019

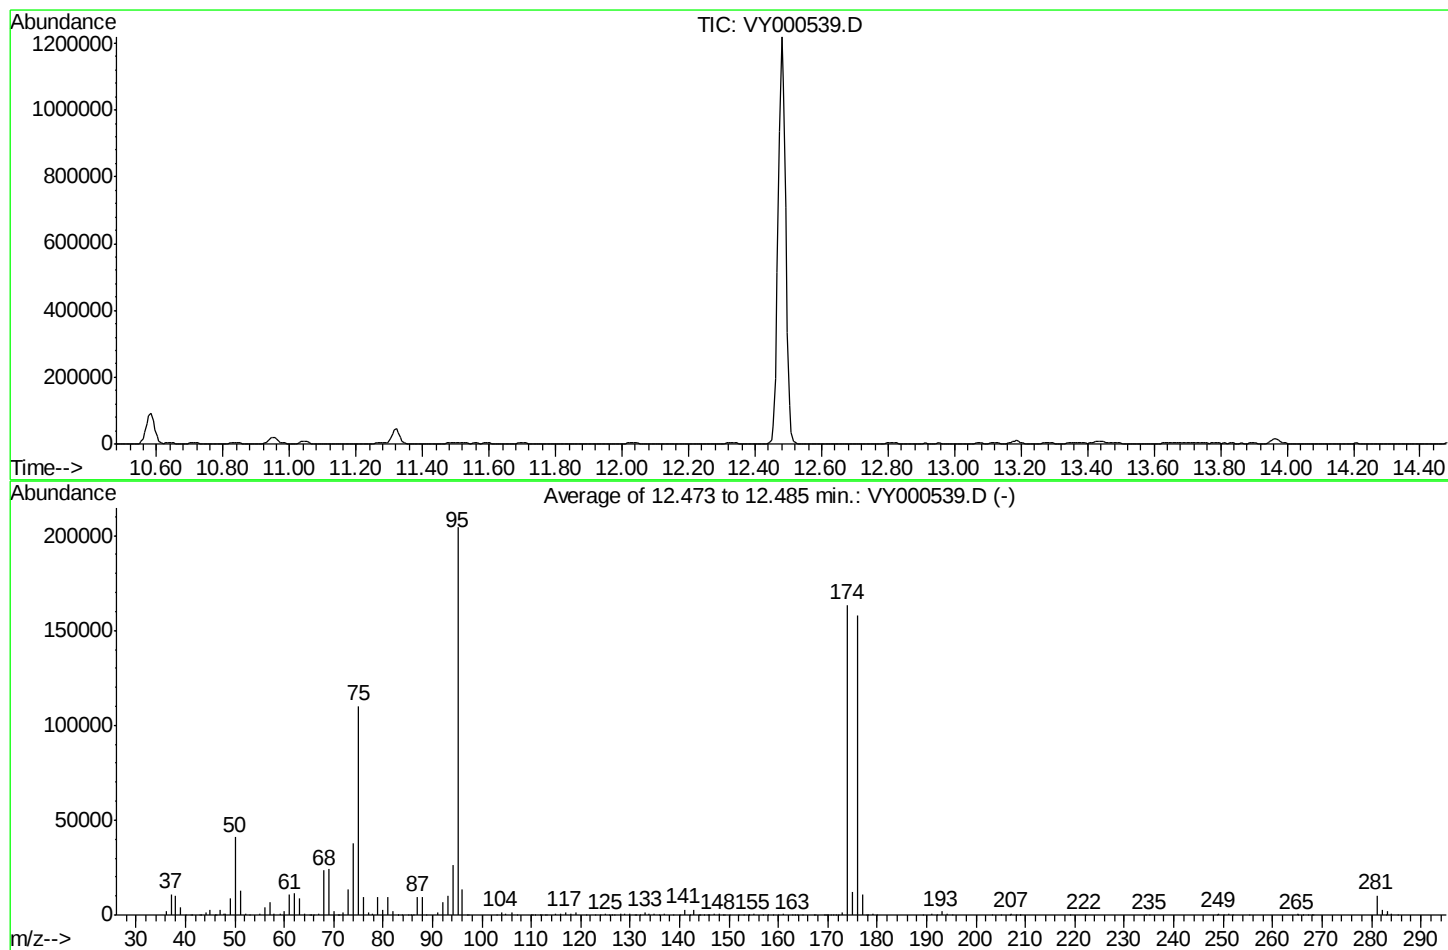

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	41146	PASS
75	95	30	60	53.8	110018	PASS
95	95	100	100	100.0	204373	PASS
96	95	5	9	6.7	13673	PASS
173	174	0.00	2	0.7	1178	PASS
174	95	50	100	80.1	163648	PASS
175	174	5	9	7.6	12410	PASS
176	174	95	101	96.6	158048	PASS
177	176	5	9	7.0	11085	PASS