

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110624\
 Data File : VY020189.D
 Acq On : 06 Nov 2024 18:13
 Operator : SY/MD
 Sample : P4707-01
 Misc : 5.01g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 HD-02-110424

Quant Time: Nov 07 00:30:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103024S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 31 15:23:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	137706	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.616	114	297134	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	284965	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	101350	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	101226	58.898	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 117.800%	
35) Dibromofluoromethane	7.634	113	101344	53.645	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 107.280%	
50) Toluene-d8	10.103	98	381210	50.694	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 101.380%	
62) 4-Bromofluorobenzene	12.402	95	113093	46.302	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	= 92.600%	


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110624\
Data File : VY020189.D
Acq On : 06 Nov 2024 18:13
Operator : SY/MD
Sample : P4707-01
Misc : 5.01g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
HD-02-110424

Quant Time: Nov 07 00:30:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103024S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 31 15:23:13 2024
Response via : Initial Calibration



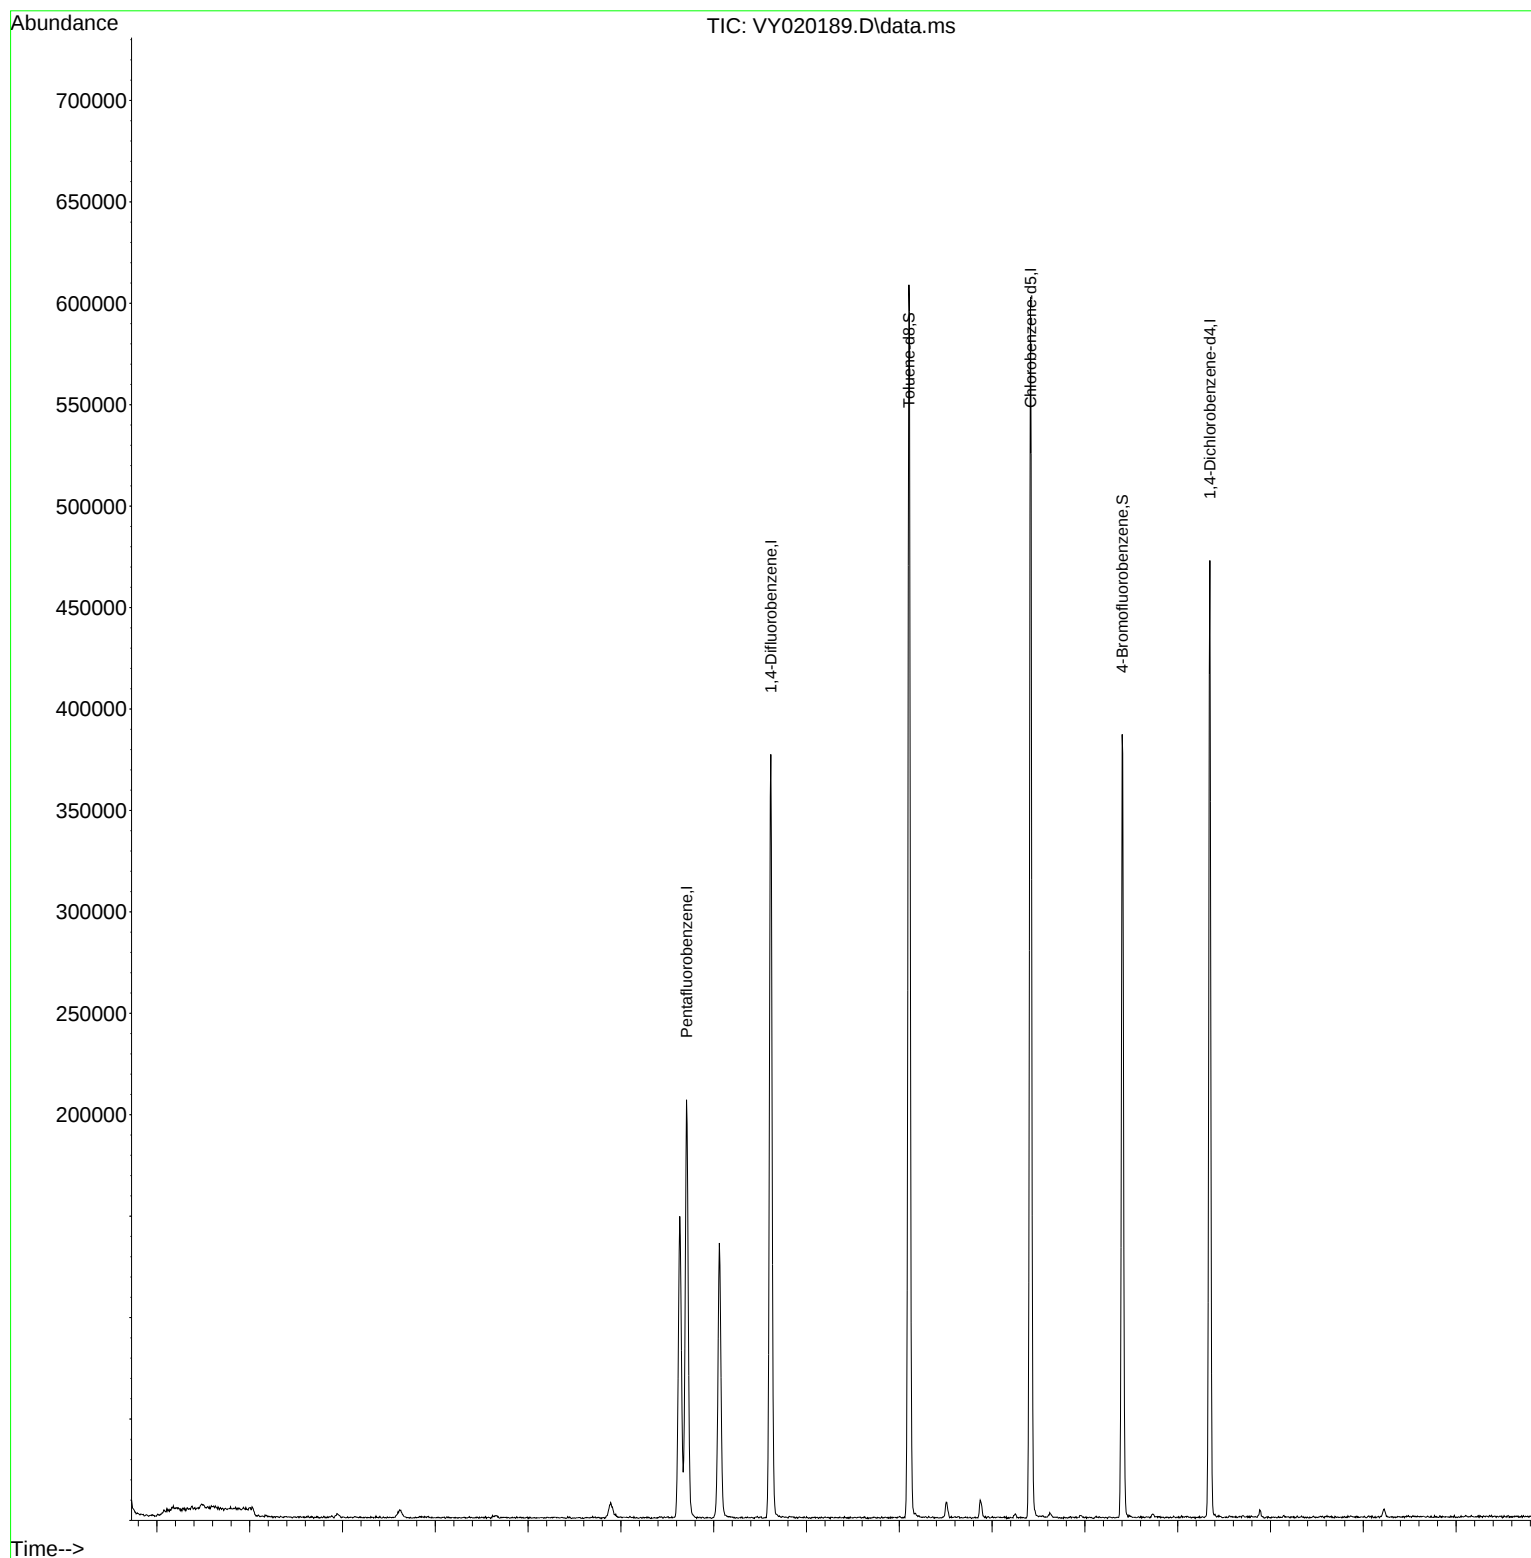




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 98
Delta R.T. 0.000 min
Lab File: VY020189.D
Acq: 06 Nov 2024 18:13




Instrument :
MSVOA_Y
ClientSampleId :
HD-02-110424


Tgt Ion:168 Resp: 137706
Ion Ratio Lower Upper
168 100
99 64.6 39.1 58.7#

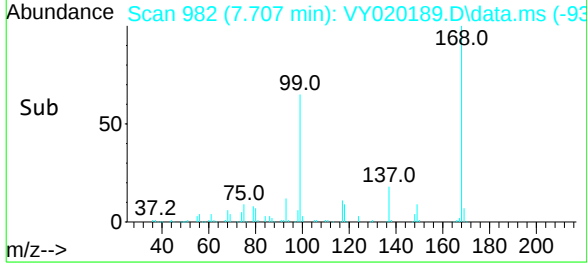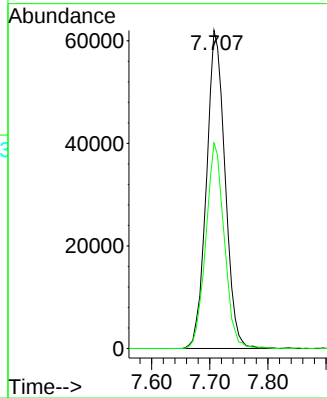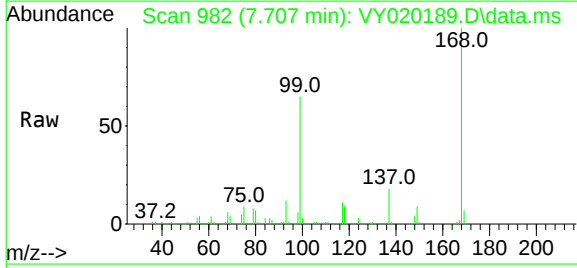

#33
1,2-Dichloroethane-d4
Concen: 58.898 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY020189.D
Acq: 06 Nov 2024 18:13

Tgt Ion: 65 Resp: 101226
Ion Ratio Lower Upper
65 100
67 52.8 0.0 109.6


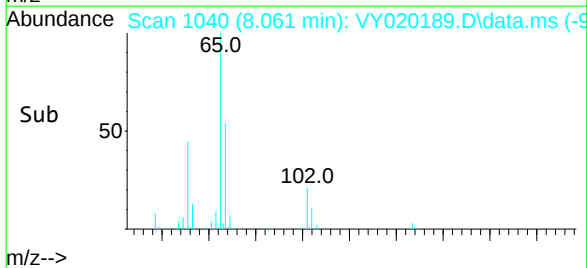
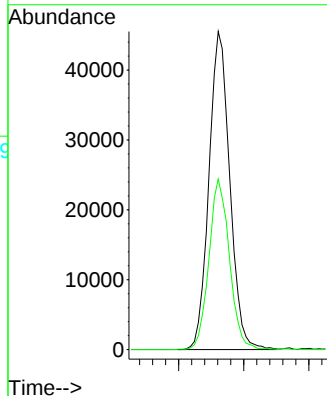
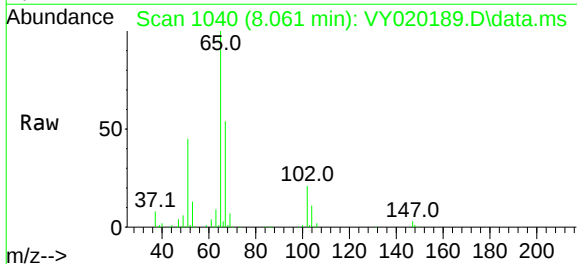


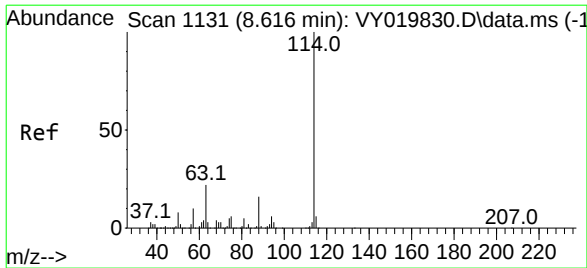

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY020189.D
Acq: 06 Nov 2024 18:13




Instrument :
MSVOA_Y
ClientSampleId :
HD-02-110424


Tgt Ion:	114	Resp:	297134
Ion	Ratio	Lower	Upper
114	100		
63	23.2	0.0	35.0
88	14.7	0.0	27.2

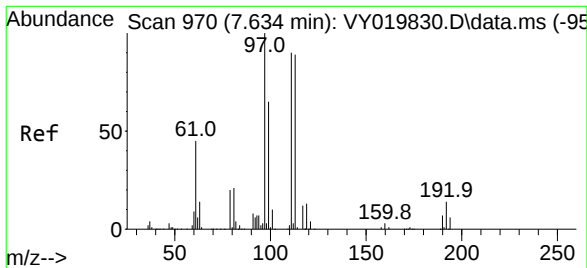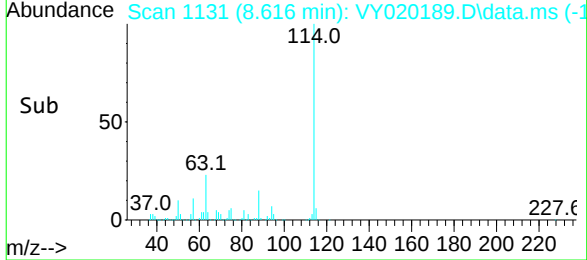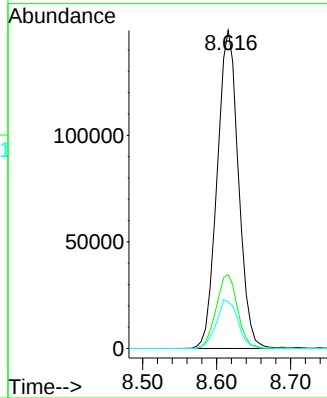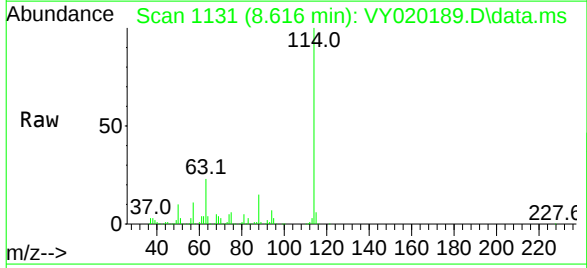

#35
Dibromofluoromethane
Concen: 53.645 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.000 min
Lab File: VY020189.D
Acq: 06 Nov 2024 18:13

Tgt Ion:	113	Resp:	101344
Ion	Ratio	Lower	Upper
113	100		
111	105.0	82.2	123.4
192	16.5	15.9	23.9

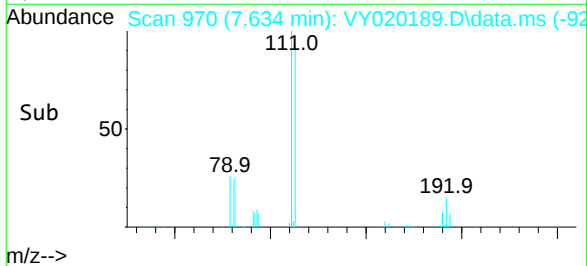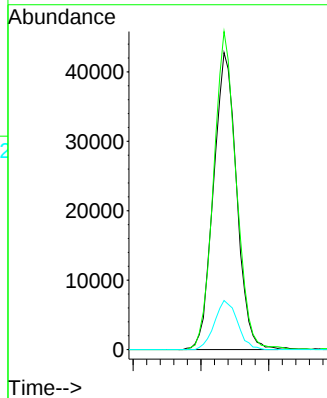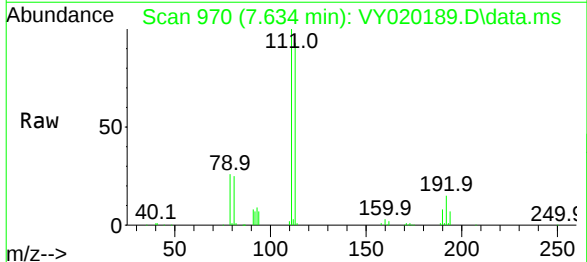

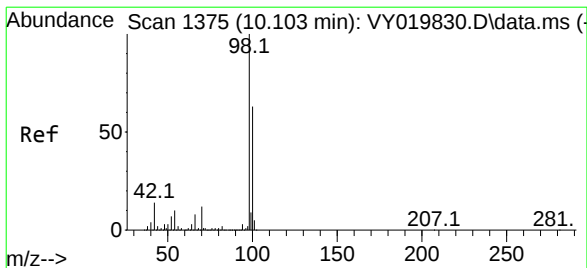

#50

Toluene-d8

Concen: 50.694 ug/l

RT: 10.103 min Scan# 1375

Delta R.T. -0.006 min

Lab File: VY020189.D

Acq: 06 Nov 2024 18:13

Instrument :

MSVOA_Y

ClientSampleId :





HD-02-110424

Tgt Ion: 98 Resp: 381210

Ion Ratio Lower Upper

98 100

100 63.7 52.0 78.0

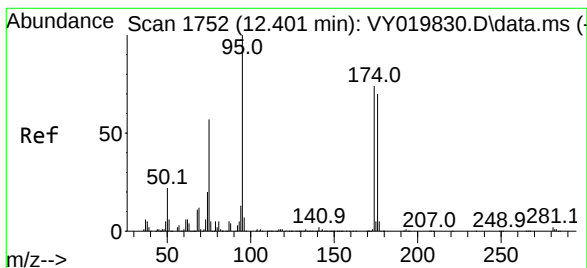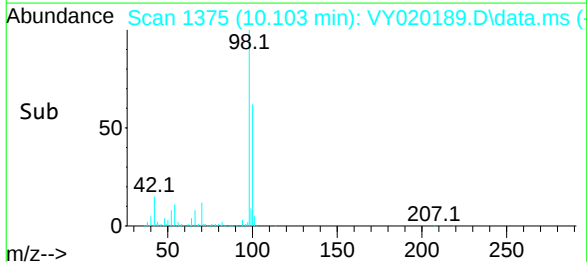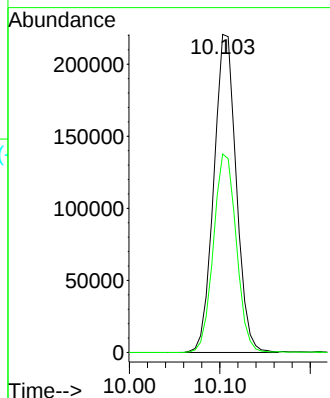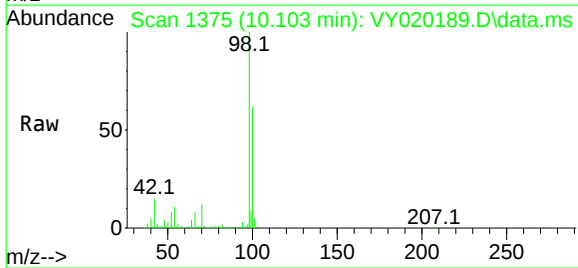

#62

4-Bromofluorobenzene

Concen: 46.302 ug/l

RT: 12.402 min Scan# 1752

Delta R.T. -0.006 min

Lab File: VY020189.D

Acq: 06 Nov 2024 18:13




Tgt Ion: 95 Resp: 113093


Ion Ratio Lower Upper

95 100

174 73.9 0.0 175.6

176 70.5 0.0 171.4

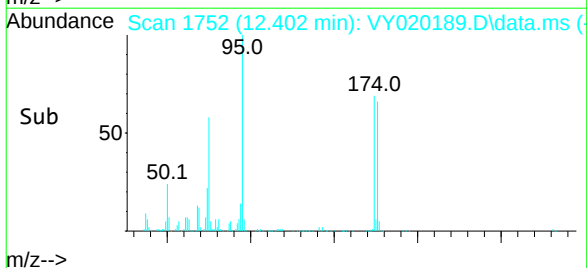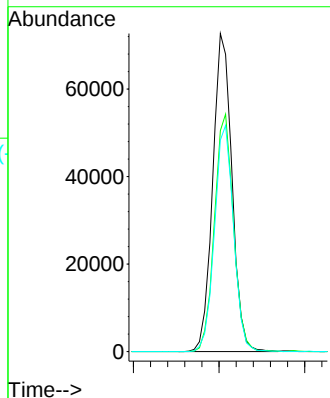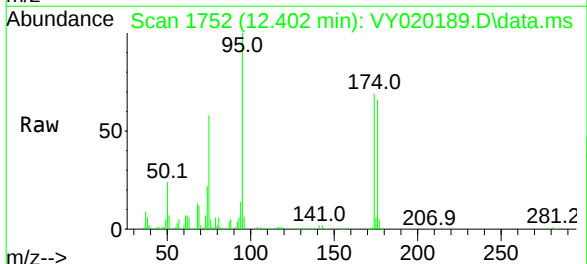

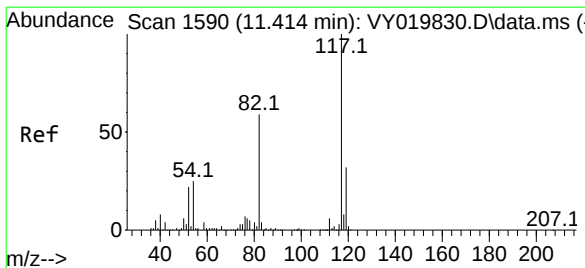

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 1590

Delta R.T. -0.006 min

Lab File: VY020189.D

Acq: 06 Nov 2024 18:13

Instrument :

MSVOA_Y

ClientSampleId :

HD-02-110424





Tgt Ion:117 Resp: 284965

Ion Ratio Lower Upper

117 100

82 60.3 42.4 63.6

119 31.5 25.9 38.9

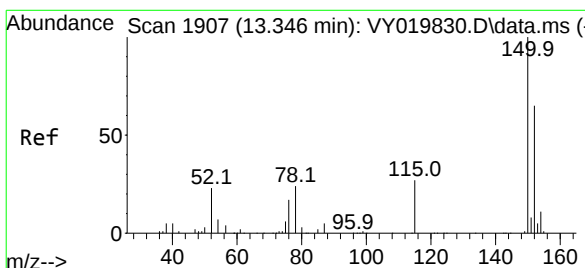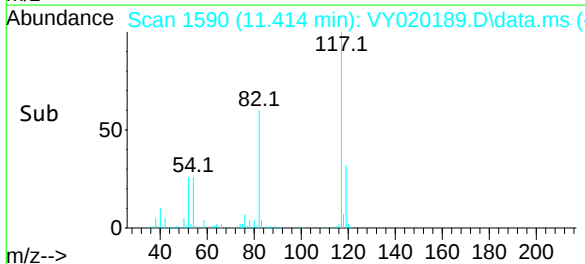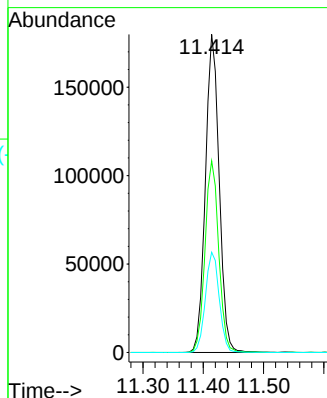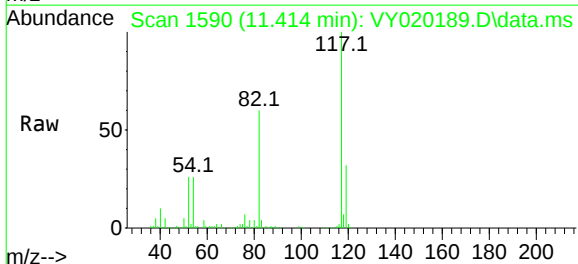

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY020189.D

Acq: 06 Nov 2024 18:13

Tgt Ion:152 Resp: 101350

Ion Ratio Lower Upper

152 100

115 62.7 28.2 84.7

150 156.2 0.0 345.6

