


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\vy110719\
Data File : VY000566.D
Acq On : 07 Nov 2019 09:17
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
Title : SW846 8260
Last Update : Wed Oct 30 13:30:53 2019

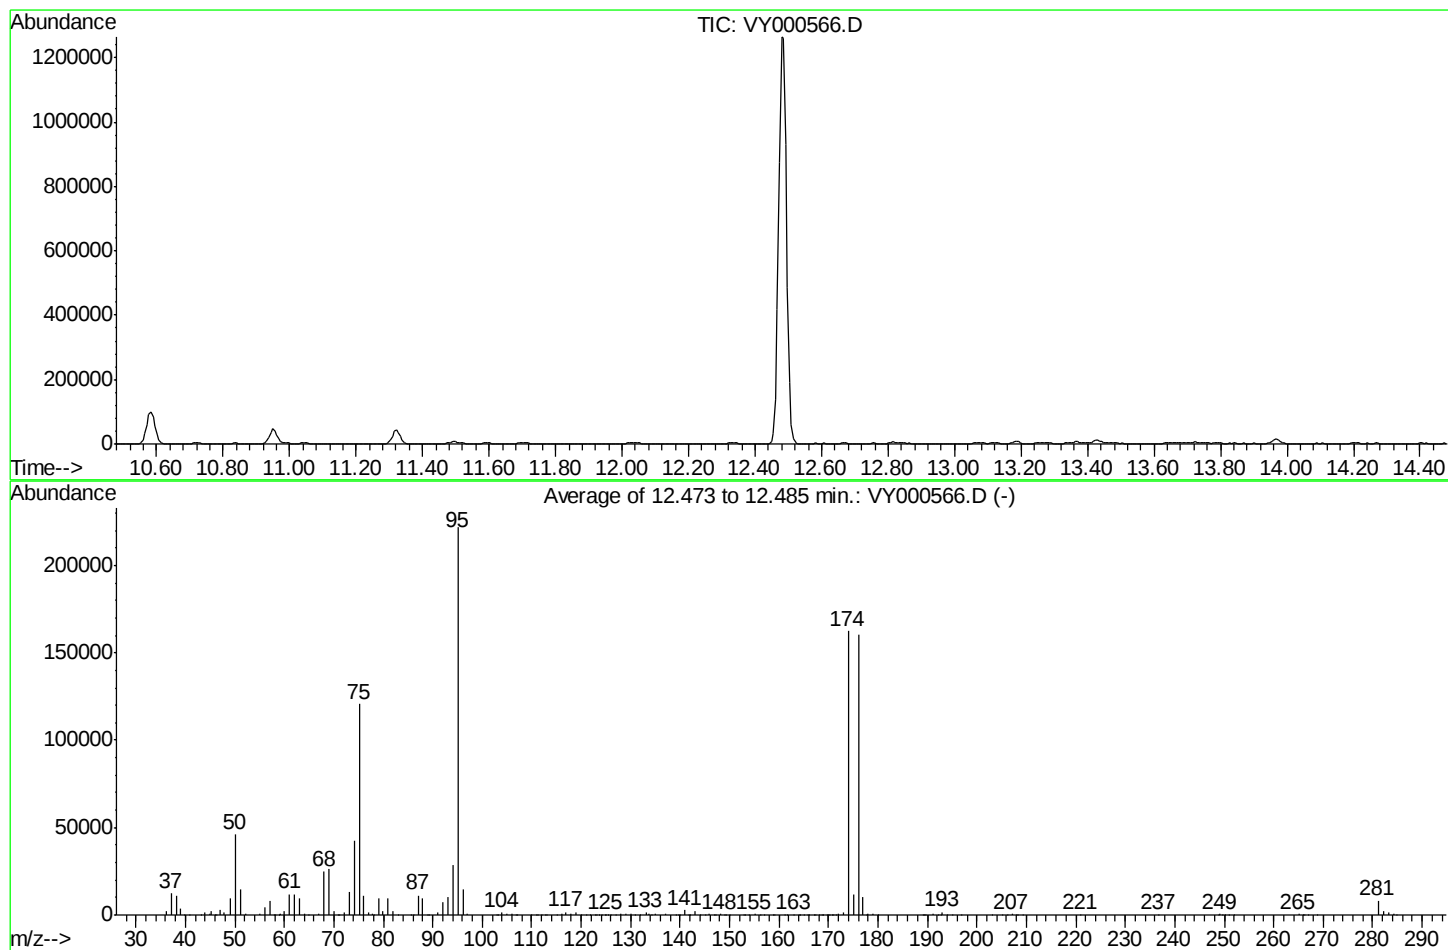

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	45826	PASS
75	95	30	60	54.5	120776	PASS
95	95	100	100	100.0	221802	PASS
96	95	5	9	6.6	14735	PASS
173	174	0.00	2	0.8	1335	PASS
174	95	50	100	73.3	162480	PASS
175	174	5	9	7.4	12011	PASS
176	174	95	101	98.8	160573	PASS
177	176	5	9	6.3	10107	PASS