


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\vy110719\
 Data File : VY000596.D
 Acq On : 07 Nov 2019 21:20
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
 Title : SW846 8260
 Last Update : Wed Oct 30 13:30:53 2019

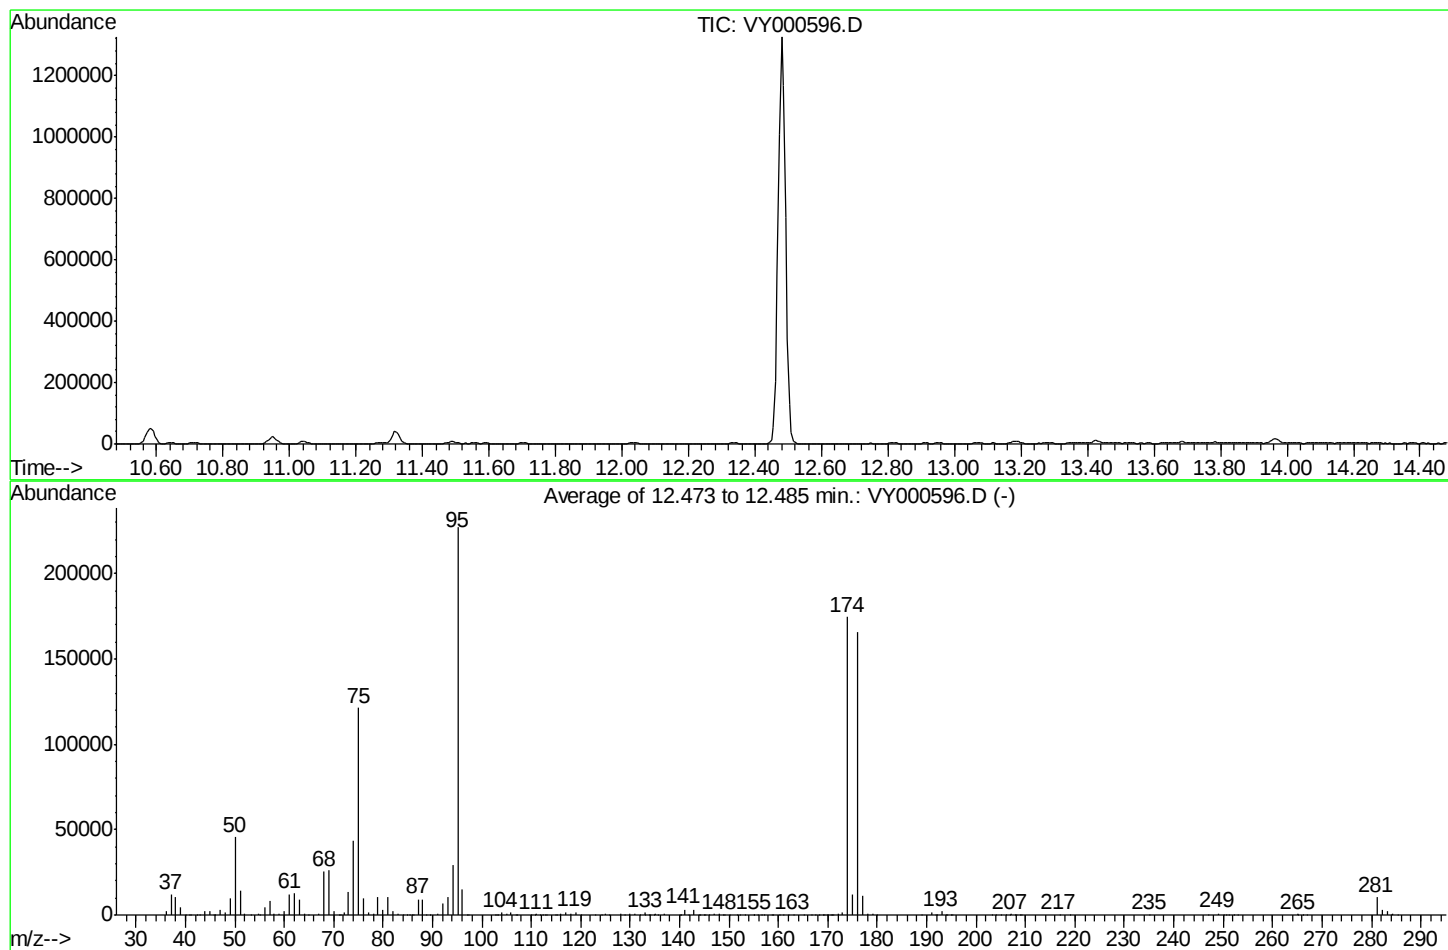

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	45522	PASS
75	95	30	60	53.4	121317	PASS
95	95	100	100	100.0	227029	PASS
96	95	5	9	6.5	14781	PASS
173	174	0.00	2	0.9	1584	PASS
174	95	50	100	76.8	174357	PASS
175	174	5	9	7.0	12285	PASS
176	174	95	101	95.0	165717	PASS
177	176	5	9	6.9	11397	PASS