
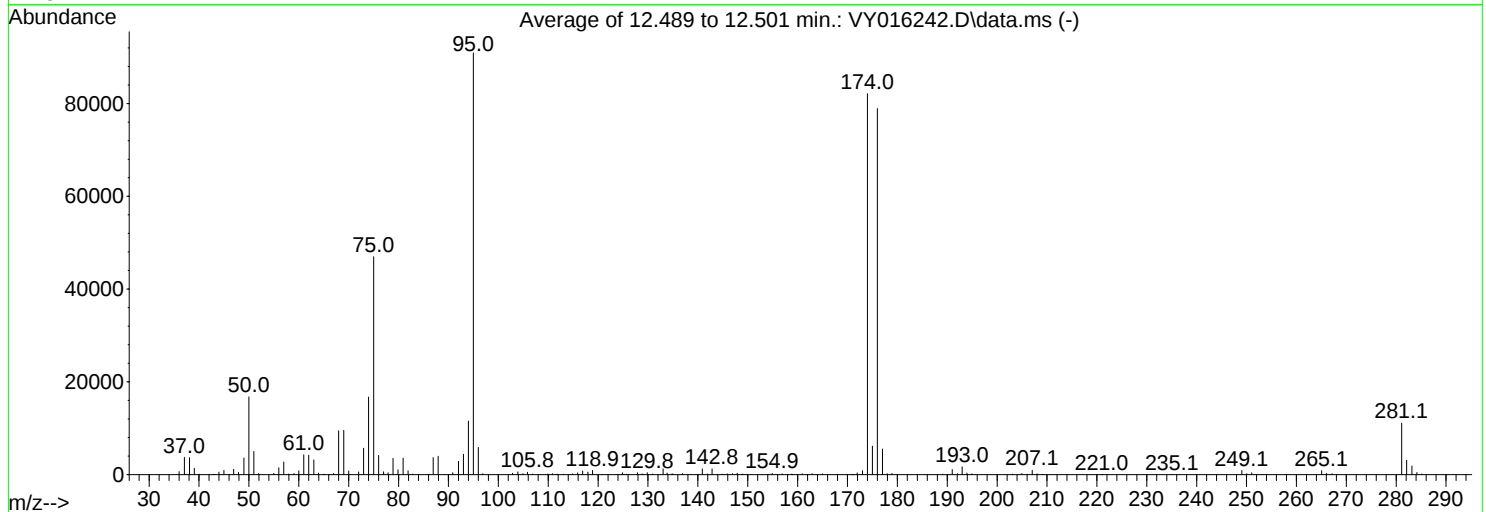


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110723\
Data File : VY016242.D
Acq On : 07 Nov 2023 08:03
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103123S.M
Title : SW846 8260
Last Update : Wed Nov 01 03:33:29 2023

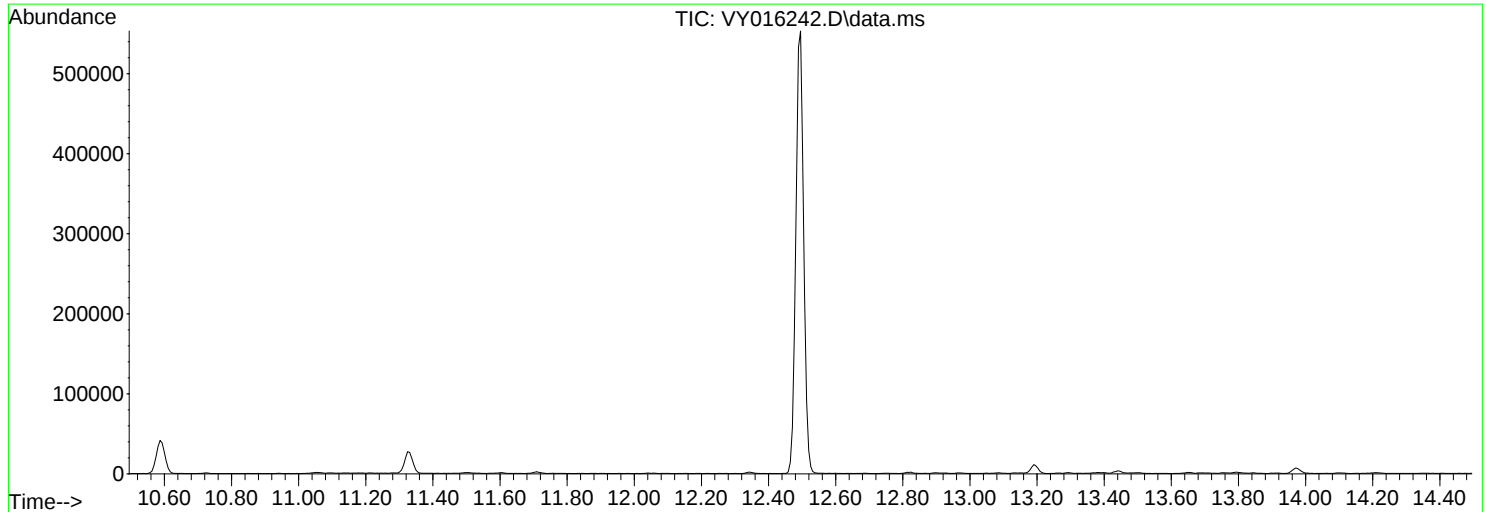

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1741

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	16764	PASS
75	95	30	60	51.7	46992	PASS
95	95	100	100	100.0	90928	PASS
96	95	5	9	6.4	5850	PASS
173	174	0.00	2	1.0	851	PASS
174	95	50	100	90.3	82109	PASS
175	174	5	9	7.5	6148	PASS
176	174	95	101	96.1	78923	PASS
177	176	5	9	7.0	5517	PASS