
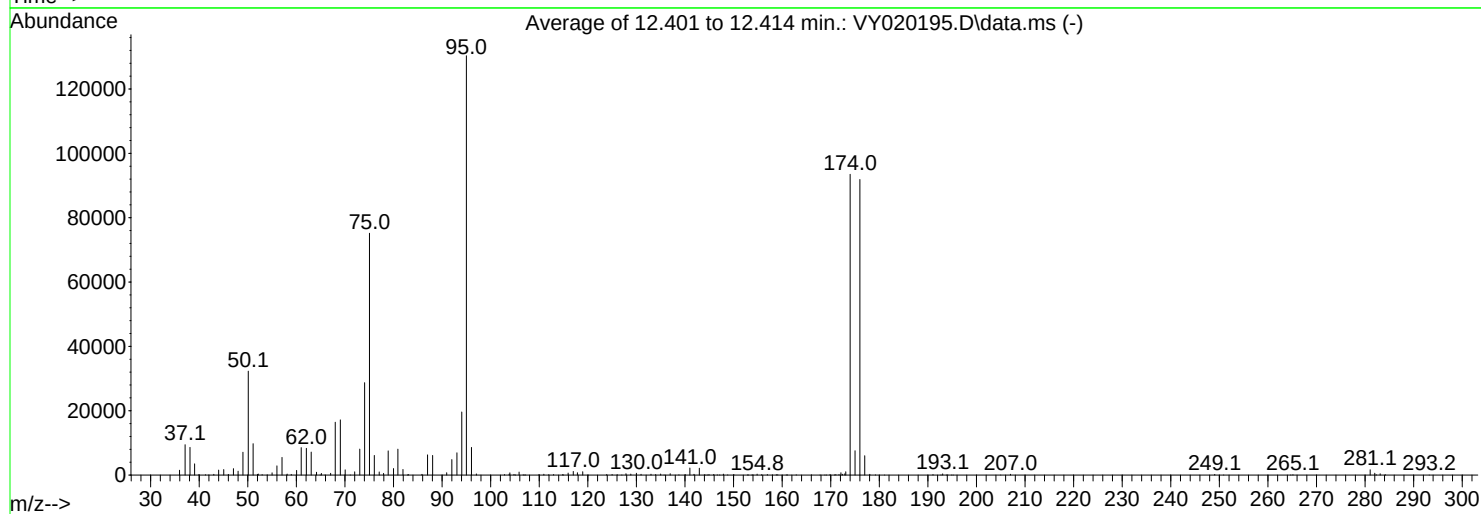


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110724\
Data File : VY020195.D
Acq On : 07 Nov 2024 08:36
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103024S.M
Title : SW846 8260
Last Update : Thu Oct 31 15:23:13 2024

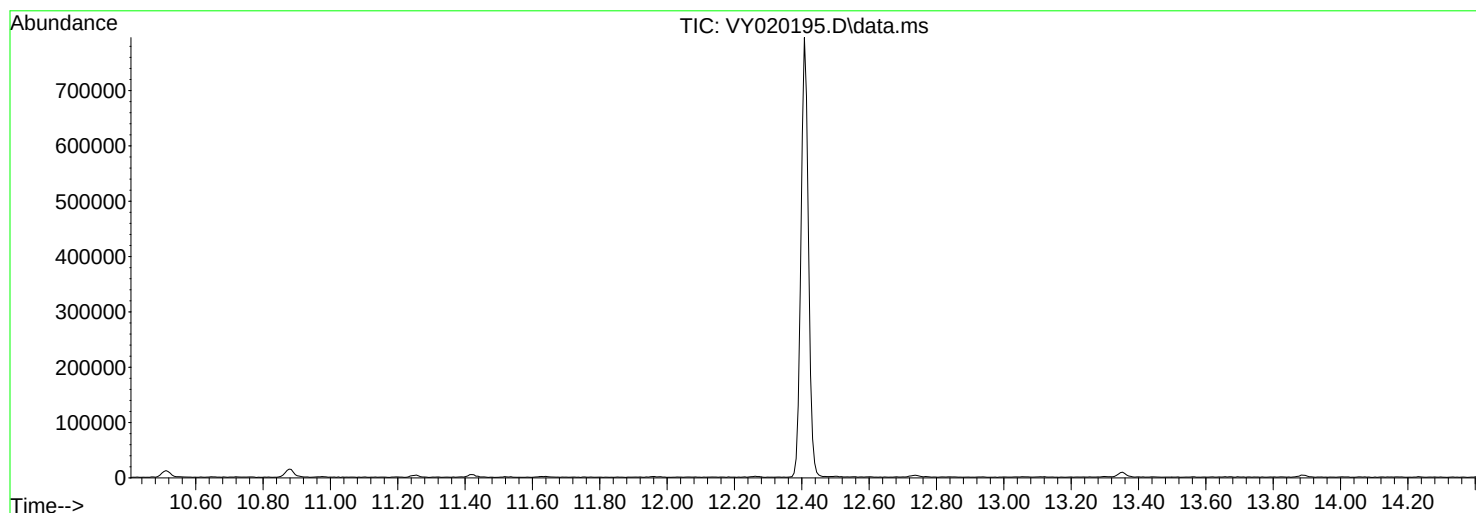

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.8	32296	PASS
75	95	30	60	57.7	75171	PASS
95	95	100	100	100.0	130347	PASS
96	95	5	9	6.6	8592	PASS
173	174	0.00	2	1.1	1033	PASS
174	95	50	100	71.7	93501	PASS
175	174	5	9	8.1	7571	PASS
176	174	95	101	98.3	91885	PASS
177	176	5	9	6.5	6014	PASS