
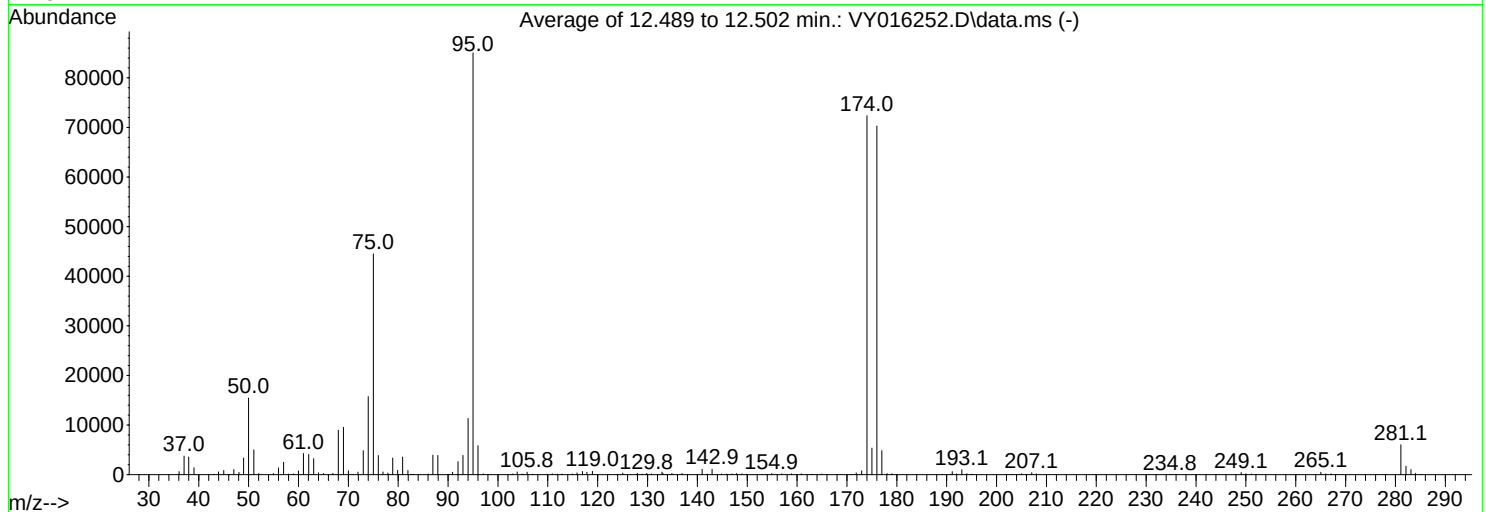


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110823\
Data File : VY016252.D
Acq On : 08 Nov 2023 07:54
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110823S.M
Title : SW846 8260
Last Update : Thu Nov 09 00:45:52 2023

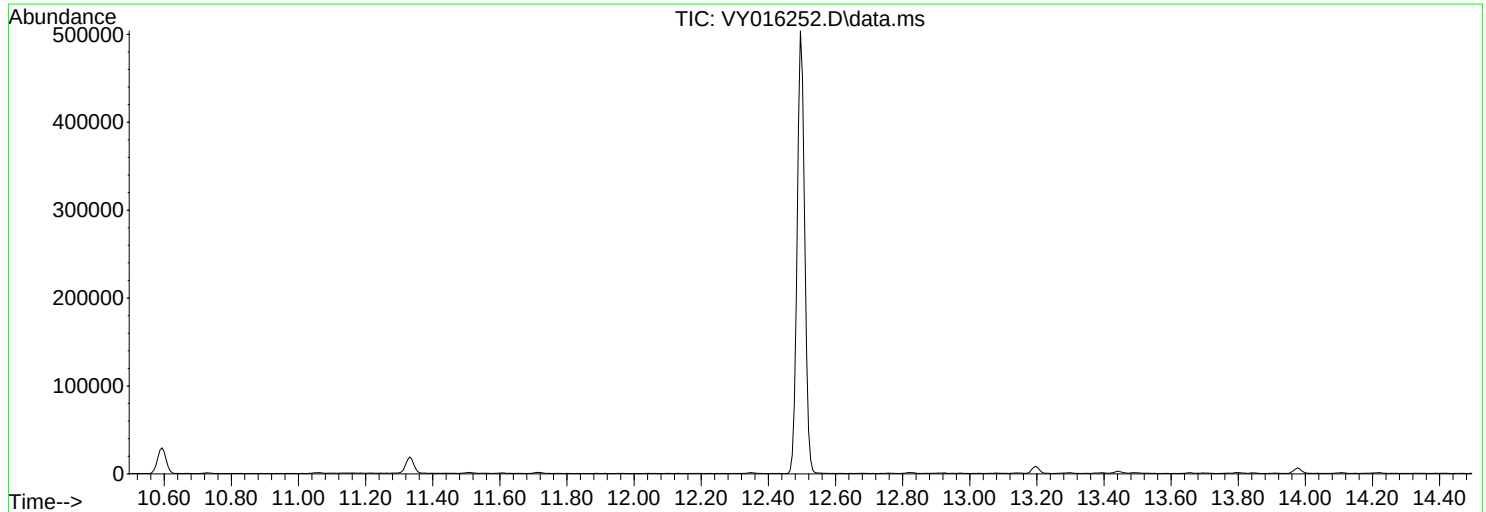

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	15450	PASS
75	95	30	60	52.4	44520	PASS
95	95	100	100	100.0	85032	PASS
96	95	5	9	6.9	5844	PASS
173	174	0.00	2	1.1	762	PASS
174	95	50	100	85.1	72341	PASS
175	174	5	9	7.4	5359	PASS
176	174	95	101	97.2	70280	PASS
177	176	5	9	6.9	4846	PASS