
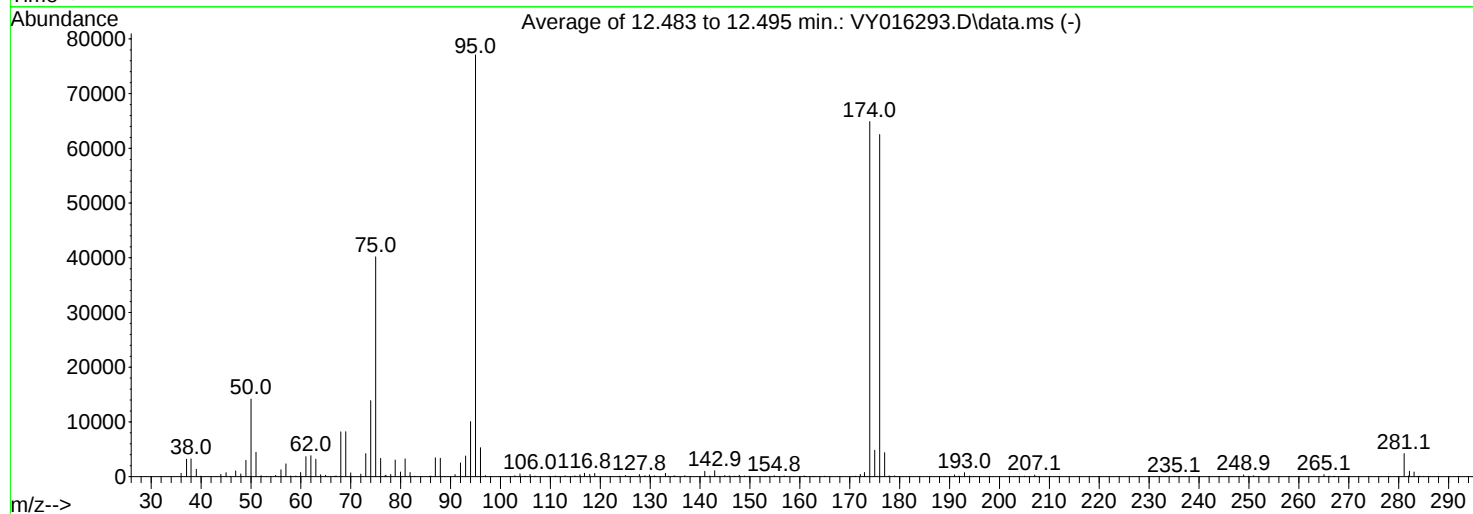


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY111023\  
Data File : VY016293.D  
Acq On : 10 Nov 2023 07:54  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y110823S.M  
Title : SW846 8260  
Last Update : Thu Nov 09 00:45:52 2023

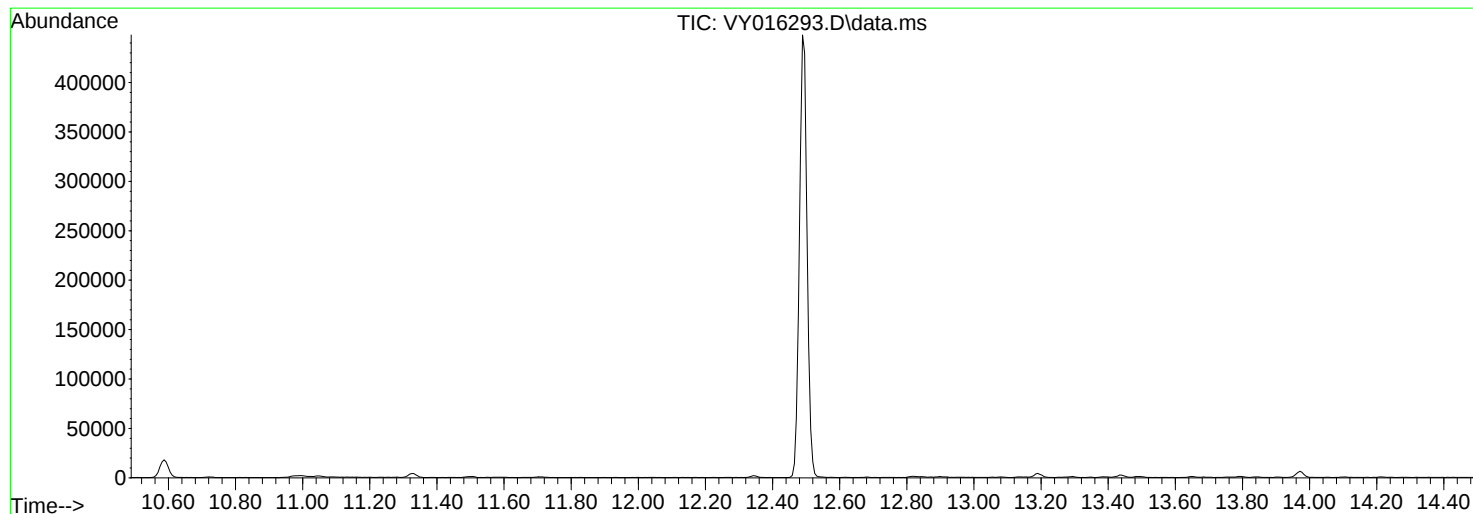

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 18.4         | 14194      | PASS                |
| 75             | 95              | 30              | 60              | 52.1         | 40168      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 77088      | PASS                |
| 96             | 95              | 5               | 9               | 6.9          | 5290       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.2          | 750        | PASS                |
| 174            | 95              | 50              | 100             | 84.2         | 64896      | PASS                |
| 175            | 174             | 5               | 9               | 7.5          | 4838       | PASS                |
| 176            | 174             | 95              | 101             | 96.3         | 62517      | PASS                |
| 177            | 176             | 5               | 9               | 7.0          | 4390       | PASS                |