

Data File : VY000652.D
Acq On : 12 Nov 2019 13:52
Operator : SY/MD
Sample : VY1112SBL01
Misc : 5.00G/10ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VBLK79

Quant Time: Nov 13 03:07:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM111219S.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 13 03:04:36 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.70	114	385468	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.49	117	351956	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.42	152	165052	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.24	65	128316	23.57	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.28%
7) Chloroethane-d5	2.76	69	113236	23.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.64%
10) 1,1-Dichloroethene-d2	3.85	63	171970	17.10	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.40%
20) 2-Butanone-d5	6.90	46	94171	41.92	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.84%
24) Chloroform-d	7.49	84	222209	21.97	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.88%
26) 1,2-Dichloroethane-d4	8.15	65	132178	22.54	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.16%
29) Benzene-d6	8.12	84	476766	23.33	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.32%
33) 1,2-Dichloropropane-d6	9.13	67	150510	23.50	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.00%
37) Toluene-d8	10.18	98	431042	22.58	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.32%
38) trans-1,3-Dichloropropene-	10.44	79	67154	22.47	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.88%
39) 2-Hexanone-d5	10.79	63	73327	42.35	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.70%
48) 1,1,2,2-Tetrachloroethane-	12.56	84	129573	20.79	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.16%
61) 1,2-Dichlorobenzene-d4	13.72	152	150546	22.81	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.24%


Target Compounds					Qvalue
25) Chloroform	7.52	83	8399	0.793 ug/L #	61
59) 1,2,3-Trichloropropane	13.42	75	24302	5.008 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VY000652.D
Acq On : 12 Nov 2019 13:52
Operator : SY/MD
Sample : VY1112SBL01
Misc : 5.00G/10ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VBLK79

Quant Time: Nov 13 03:07:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOM2YLM111219S.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 13 03:04:36 2019
Response via : Initial Calibration

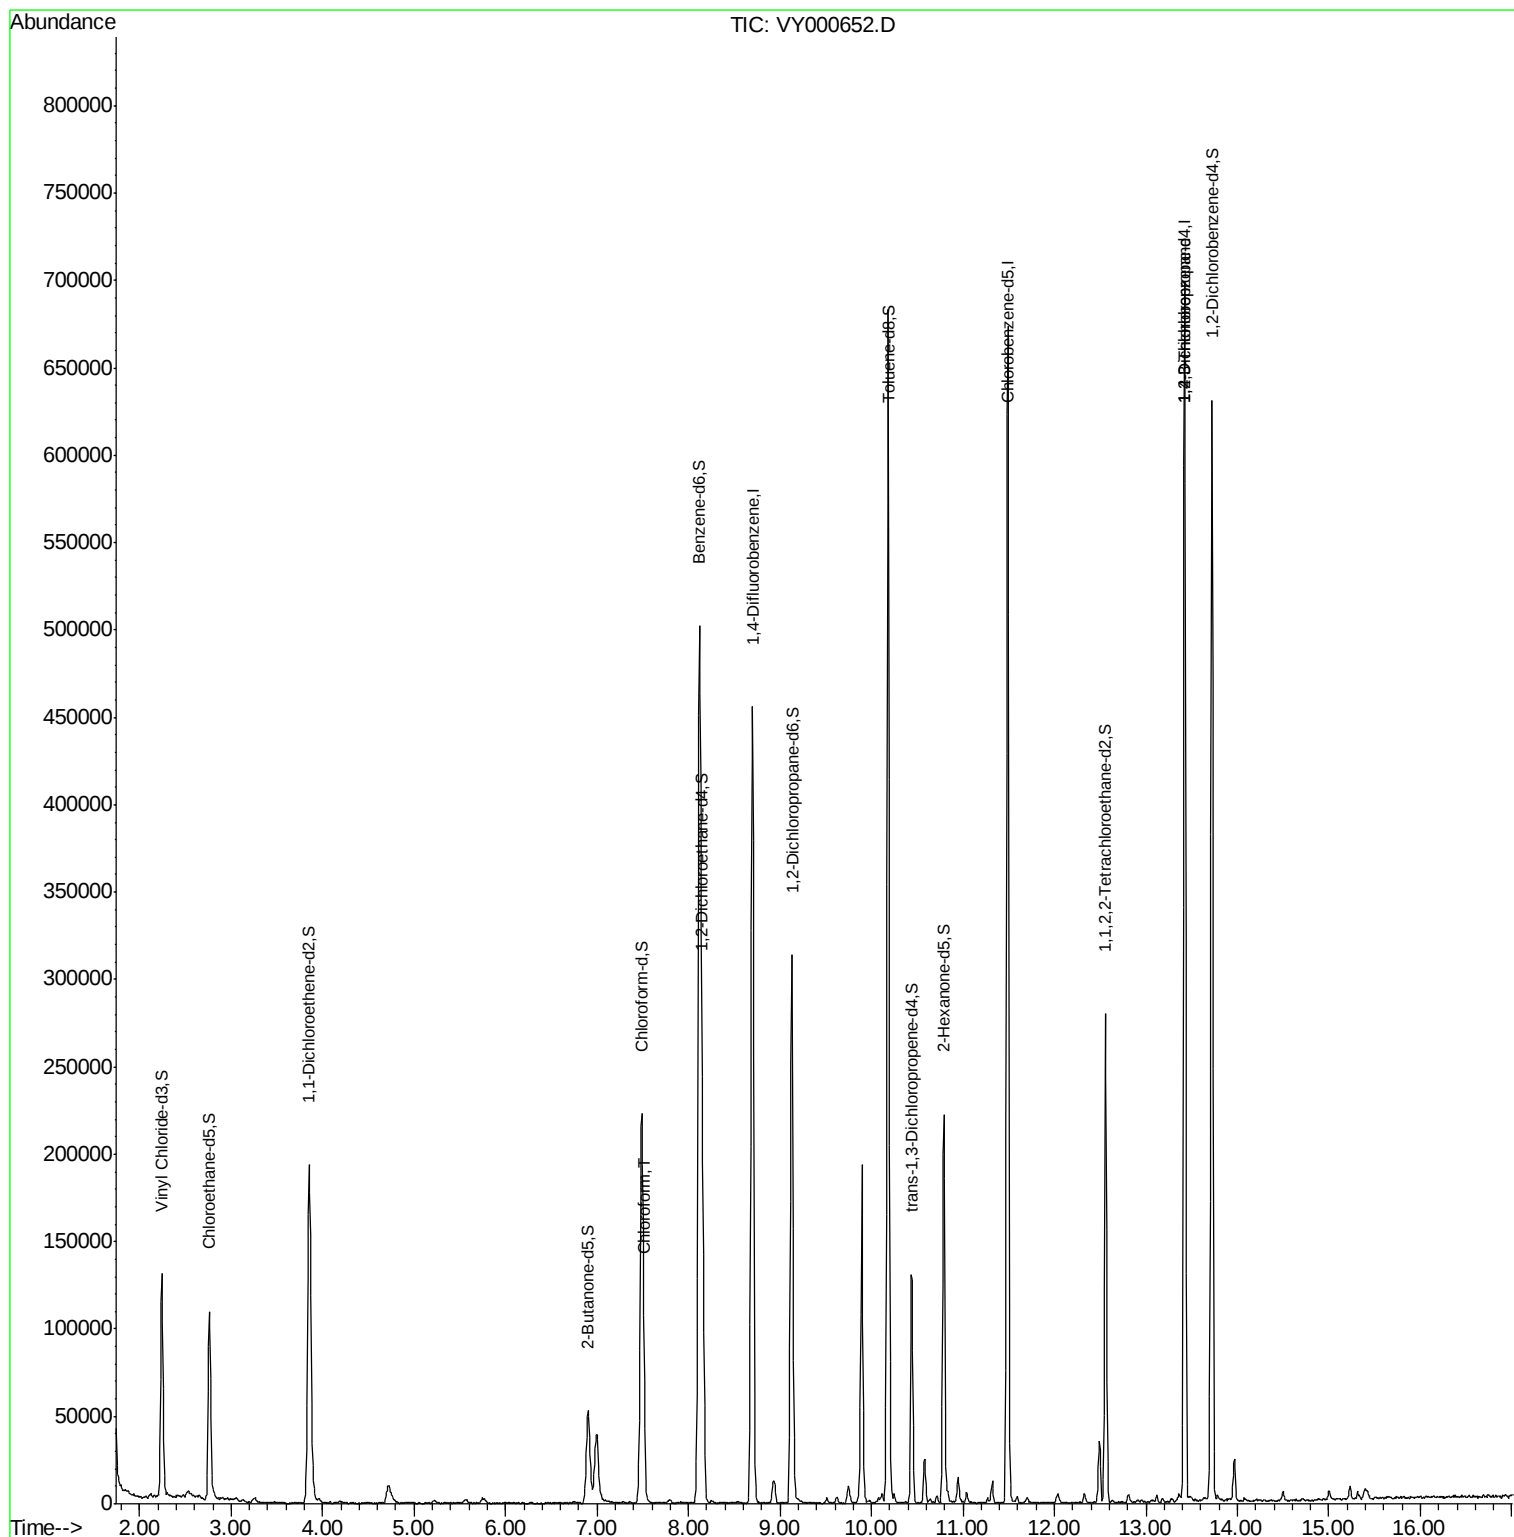

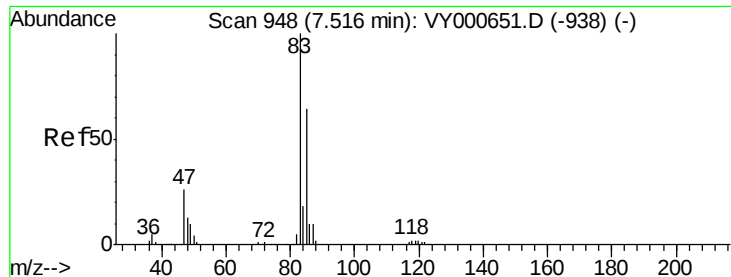

#25

Chloroform

Concen: 0.793 ug/L

RT: 7.52 min Scan# 948

Delta R.T. 0.00 min

Lab File: VY000652.D

Acq: 12 Nov 2019 13:52

Instrument :

MSVOA_Y

ClientSampleId :





VBLK79

Tgt Ion: 83 Resp: 8399

Ion Ratio Lower Upper

83 100

85 96.2 45.6 84.6#

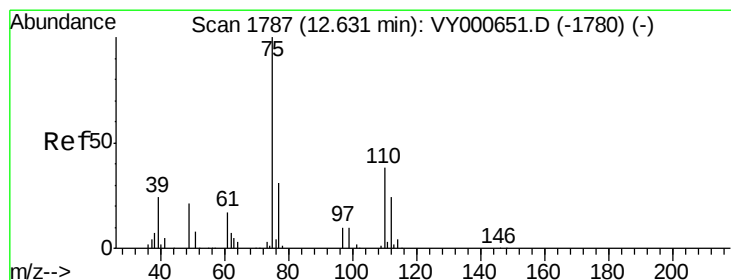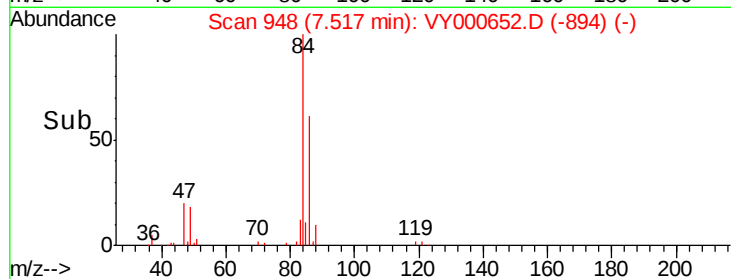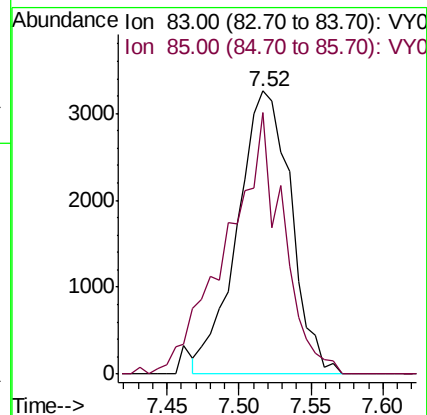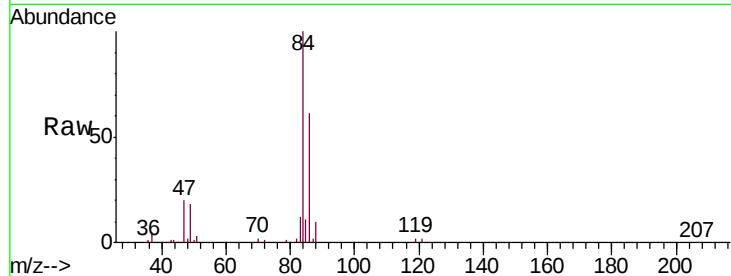

#59

1,2,3-Trichloropropane

Concen: 5.008 ug/L

RT: 13.42 min Scan# 1917

Delta R.T. 0.79 min

Lab File: VY000652.D

Acq: 12 Nov 2019 13:52

Tgt Ion: 75 Resp: 24302

Ion Ratio Lower Upper

75 100

77 35.0 26.4 39.6

