
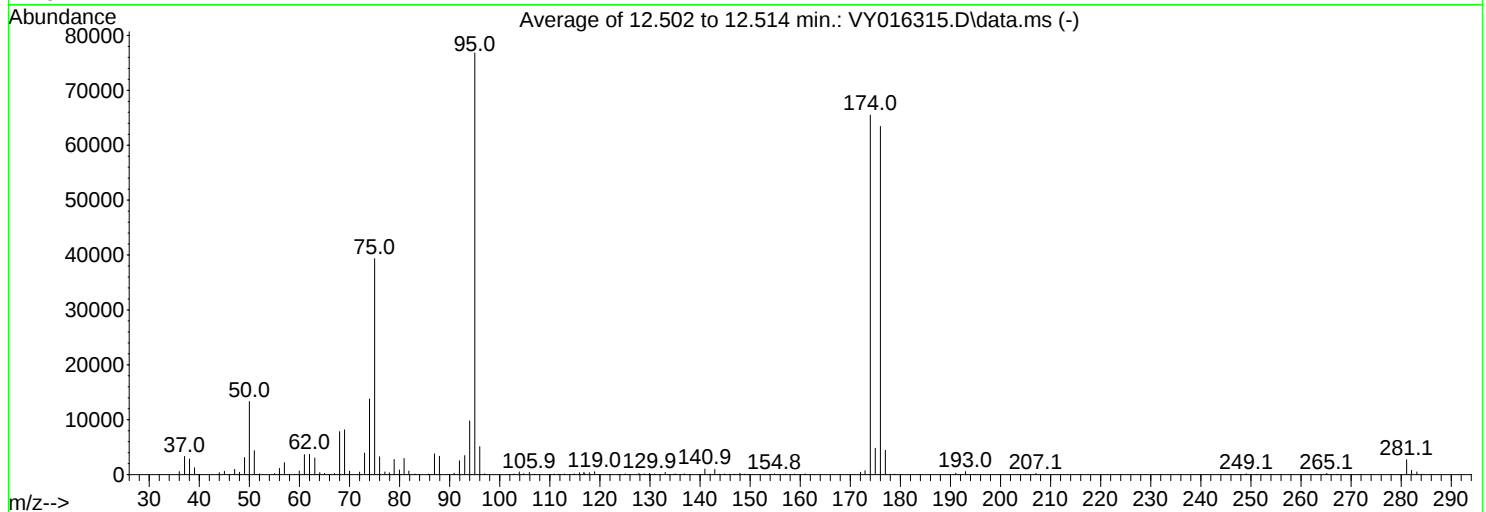


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY111323\
Data File : VY016315.D
Acq On : 13 Nov 2023 07:57
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110823S.M
Title : SW846 8260
Last Update : Thu Nov 09 00:45:52 2023

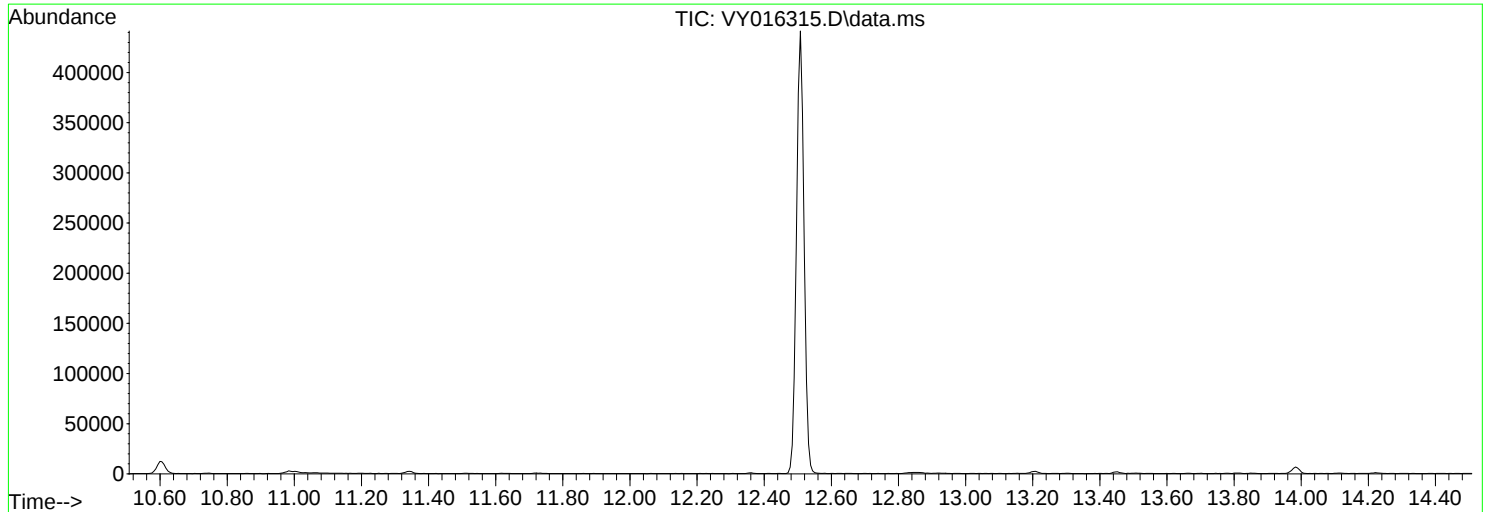

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	13314	PASS
75	95	30	60	51.2	39344	PASS
95	95	100	100	100.0	76827	PASS
96	95	5	9	6.6	5106	PASS
173	174	0.00	2	1.1	733	PASS
174	95	50	100	85.3	65499	PASS
175	174	5	9	7.3	4812	PASS
176	174	95	101	96.8	63408	PASS
177	176	5	9	7.0	4445	PASS