


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv111419\
Data File : VY000672.D
Acq On : 14 Nov 2019 10:26
Operator : SY/MD
Sample : BFB81
Misc : 5ML/MSVOA Y/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB81

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SOMYLM111419WMA.M
Title : VOC Analysis
Last Update : Fri Nov 15 12:09:40 2019

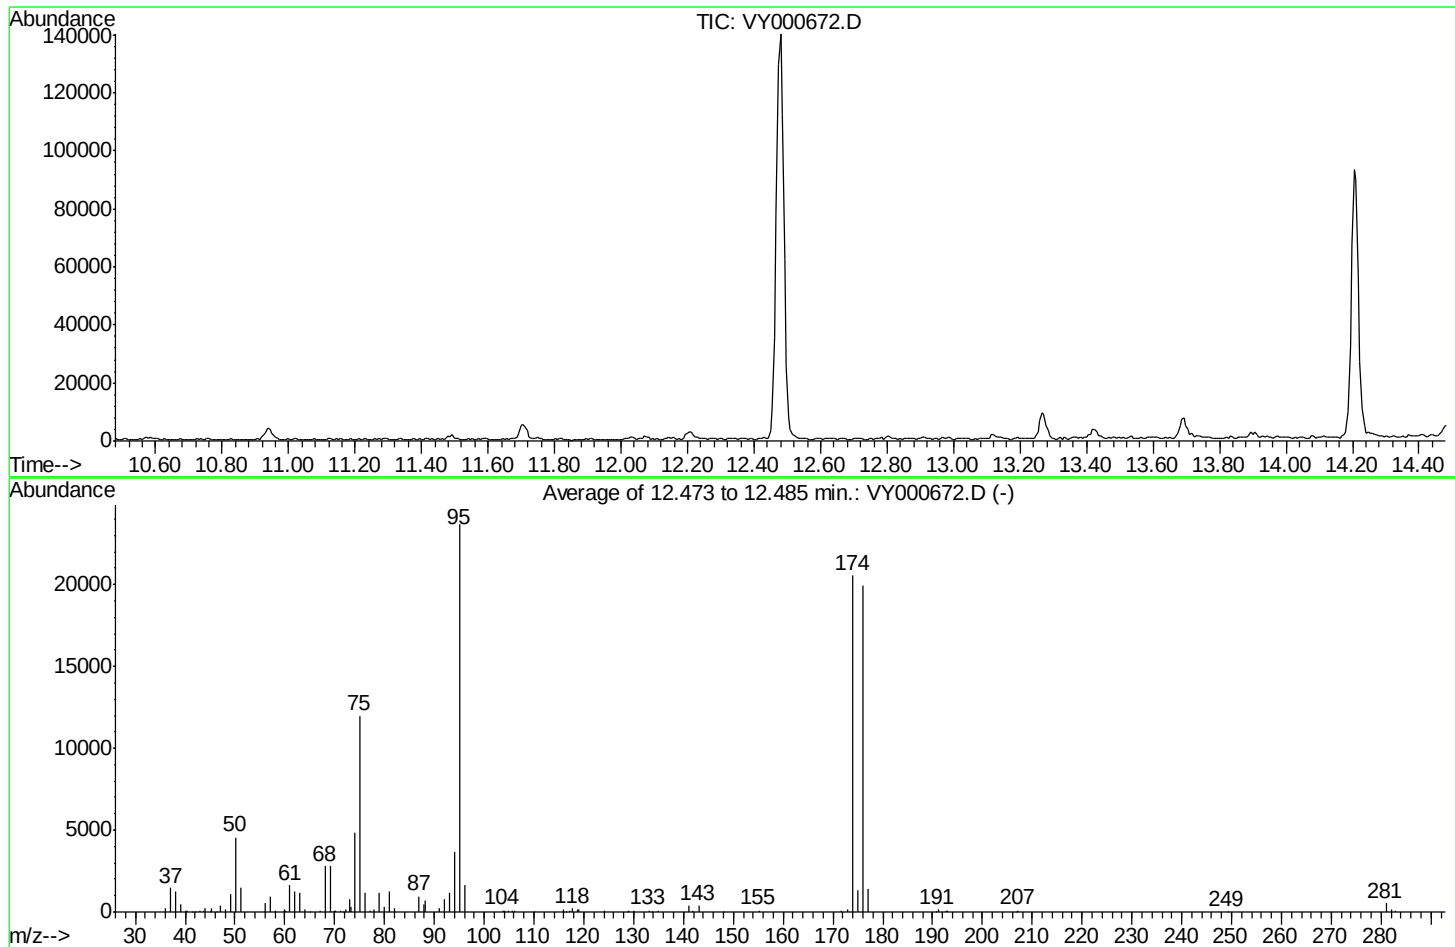

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1755

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	4552	PASS
75	95	30	80	50.6	11985	PASS
95	95	100	100	100.0	23677	PASS
96	95	5	9	6.9	1637	PASS
173	174	0.00	2	0.7	143	PASS
174	95	50	120	86.7	20536	PASS
175	174	5	9	6.6	1359	PASS
176	174	95	101	97.2	19962	PASS
177	176	5	9	7.0	1391	PASS

m/z	Abundance
36.00	203.0
37.00	1339.0
38.20	1097.0
39.10	569.0
40.00	168.0
41.30	93.0
43.10	73.0
43.80	321.0
44.10	369.0
45.10	401.0
46.20	72.0
47.10	459.0
49.10	1446.0
50.10	5430.0
51.10	1844.0
56.10	519.0
57.00	1164.0
58.10	87.0
60.10	216.0
61.10	2076.0
62.00	1283.0
63.10	1179.0
64.10	220.0
65.00	80.0
67.10	95.0
68.00	3215.0
69.00	3086.0
69.80	99.0
71.70	84.0
72.20	126.0
73.00	1078.0
74.00	5257.0
75.10	12774.0
76.10	1373.0
77.00	209.0
78.00	191.0
78.90	1538.0
79.90	386.0
81.00	1109.0
82.10	178.0
87.00	951.0
87.90	1317.0
91.10	396.0
91.90	948.0
93.00	1083.0
94.10	3973.0
95.10	24408.0
96.10	1574.0
103.70	111.0
104.80	71.0
105.70	217.0
115.80	72.0
116.30	112.0
117.80	294.0
118.70	301.0
119.20	276.0
130.00	87.0
133.00	81.0
135.00	56.0
141.00	471.0
141.80	95.0
143.10	304.0
155.10	108.0
172.80	159.0
174.00	18960.0
175.00	1592.0
176.00	18128.0
177.00	1473.0
190.70	73.0
191.20	165.0
192.80	97.0
206.90	93.0
281.00	296.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB81

m/z	Abundance
36.00	288.0
37.10	1780.0
38.00	1394.0
39.10	459.0
40.30	229.0
43.20	133.0
44.00	533.0
45.20	237.0
47.00	465.0
48.10	262.0
49.10	1013.0
50.10	4799.0
51.10	1587.0
56.00	512.0
57.10	980.0
58.00	157.0
59.90	291.0
61.10	1523.0
62.10	1179.0
63.10	1213.0
64.10	100.0
67.20	65.0
68.00	2667.0
69.10	3606.0
70.10	337.0
71.20	82.0
72.20	268.0
73.00	1214.0
74.00	4920.0
75.00	13484.0
76.10	1151.0
77.20	140.0
77.90	178.0
78.90	1108.0
80.00	395.0
80.90	1516.0
82.00	303.0
87.00	1117.0
88.10	1385.0
91.00	245.0
92.00	791.0
93.00	1586.0
94.10	4404.0
95.10	26416.0
96.00	2179.0
103.70	177.0
104.90	53.0
106.00	128.0
116.00	150.0
117.10	82.0
117.80	214.0
118.80	144.0
124.10	64.0
128.70	83.0
129.10	72.0
130.00	125.0
133.00	121.0
135.00	132.0
141.00	238.0
141.80	97.0
143.00	393.0
148.00	66.0
155.10	147.0
171.80	67.0
173.00	237.0
174.00	22200.0
175.10	1387.0
176.00	22568.0
177.10	1190.0
191.10	216.0
193.10	153.0
207.10	137.0
249.10	50.0
281.10	712.0
282.20	191.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB81

m/z	Abundance
36.10	142.0
37.10	1286.0
38.10	1236.0
39.10	478.0
40.10	181.0
40.90	164.0
41.80	78.0
42.90	242.0
44.00	663.0
44.90	118.0
47.00	216.0
48.10	205.0
49.00	861.0
50.10	3428.0
51.00	1119.0
55.90	237.0
56.20	287.0
57.00	669.0
60.20	272.0
61.00	1268.0
62.10	1282.0
63.00	1098.0
64.20	82.0
68.00	2485.0
69.10	2080.0
69.90	232.0
71.00	57.0
73.20	994.0
74.10	4397.0
75.10	9697.0
76.00	985.0
77.10	198.0
77.90	73.0
79.00	921.0
80.10	228.0
80.90	1064.0
82.00	210.0
86.90	840.0
88.00	757.0
91.00	164.0
92.10	600.0
93.00	822.0
94.10	2730.0
95.10	20208.0
96.10	1158.0
104.00	138.0
105.00	54.0
106.10	93.0
110.00	54.0
116.00	227.0
117.20	89.0
117.90	120.0
119.00	206.0
124.10	88.0
129.10	60.0
133.00	88.0
133.60	63.0
141.10	405.0
143.10	458.0
171.70	117.0
173.10	193.0
174.00	20448.0
174.90	1099.0
176.00	19192.0
177.00	1511.0
192.70	69.0
193.00	67.0
207.20	118.0
281.10	617.0
282.10	360.0
282.90	157.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB81

Scan 1755 (12.437 min): VY000672.D
BFB81

m/z	Abundance
39.80	191.0
40.90	75.0
43.30	170.0
44.00	280.0
69.20	75.0
76.90	92.0
114.00	53.0
163.10	78.0

Instrument :
MSVOA_Y
ClientSampleId :
BFB81