

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_Y\DATA\VY111519\
 Data File : VY000707.D
 Acq On : 15 Nov 2019 17:27
 Operator : SY/MD
 Sample : K5861-18
 Misc : 4.42G/5ML/MSVOA_Y/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 EP-15

Quant Time: Nov 16 02:33:01 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 30 13:30:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.80
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.70
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.49
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.42
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	12.70	95	46	0.00	ug/l	0.22
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_Y\DATA\VY111519\
Data File : VY000707.D
Acq On : 15 Nov 2019 17:27
Operator : SY/MD
Sample : K5861-18
Misc : 4.42G/5ML/MSVOA_Y/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
EP-15

Quant Time: Nov 16 02:33:01 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 30 13:30:53 2019
Response via : Initial Calibration

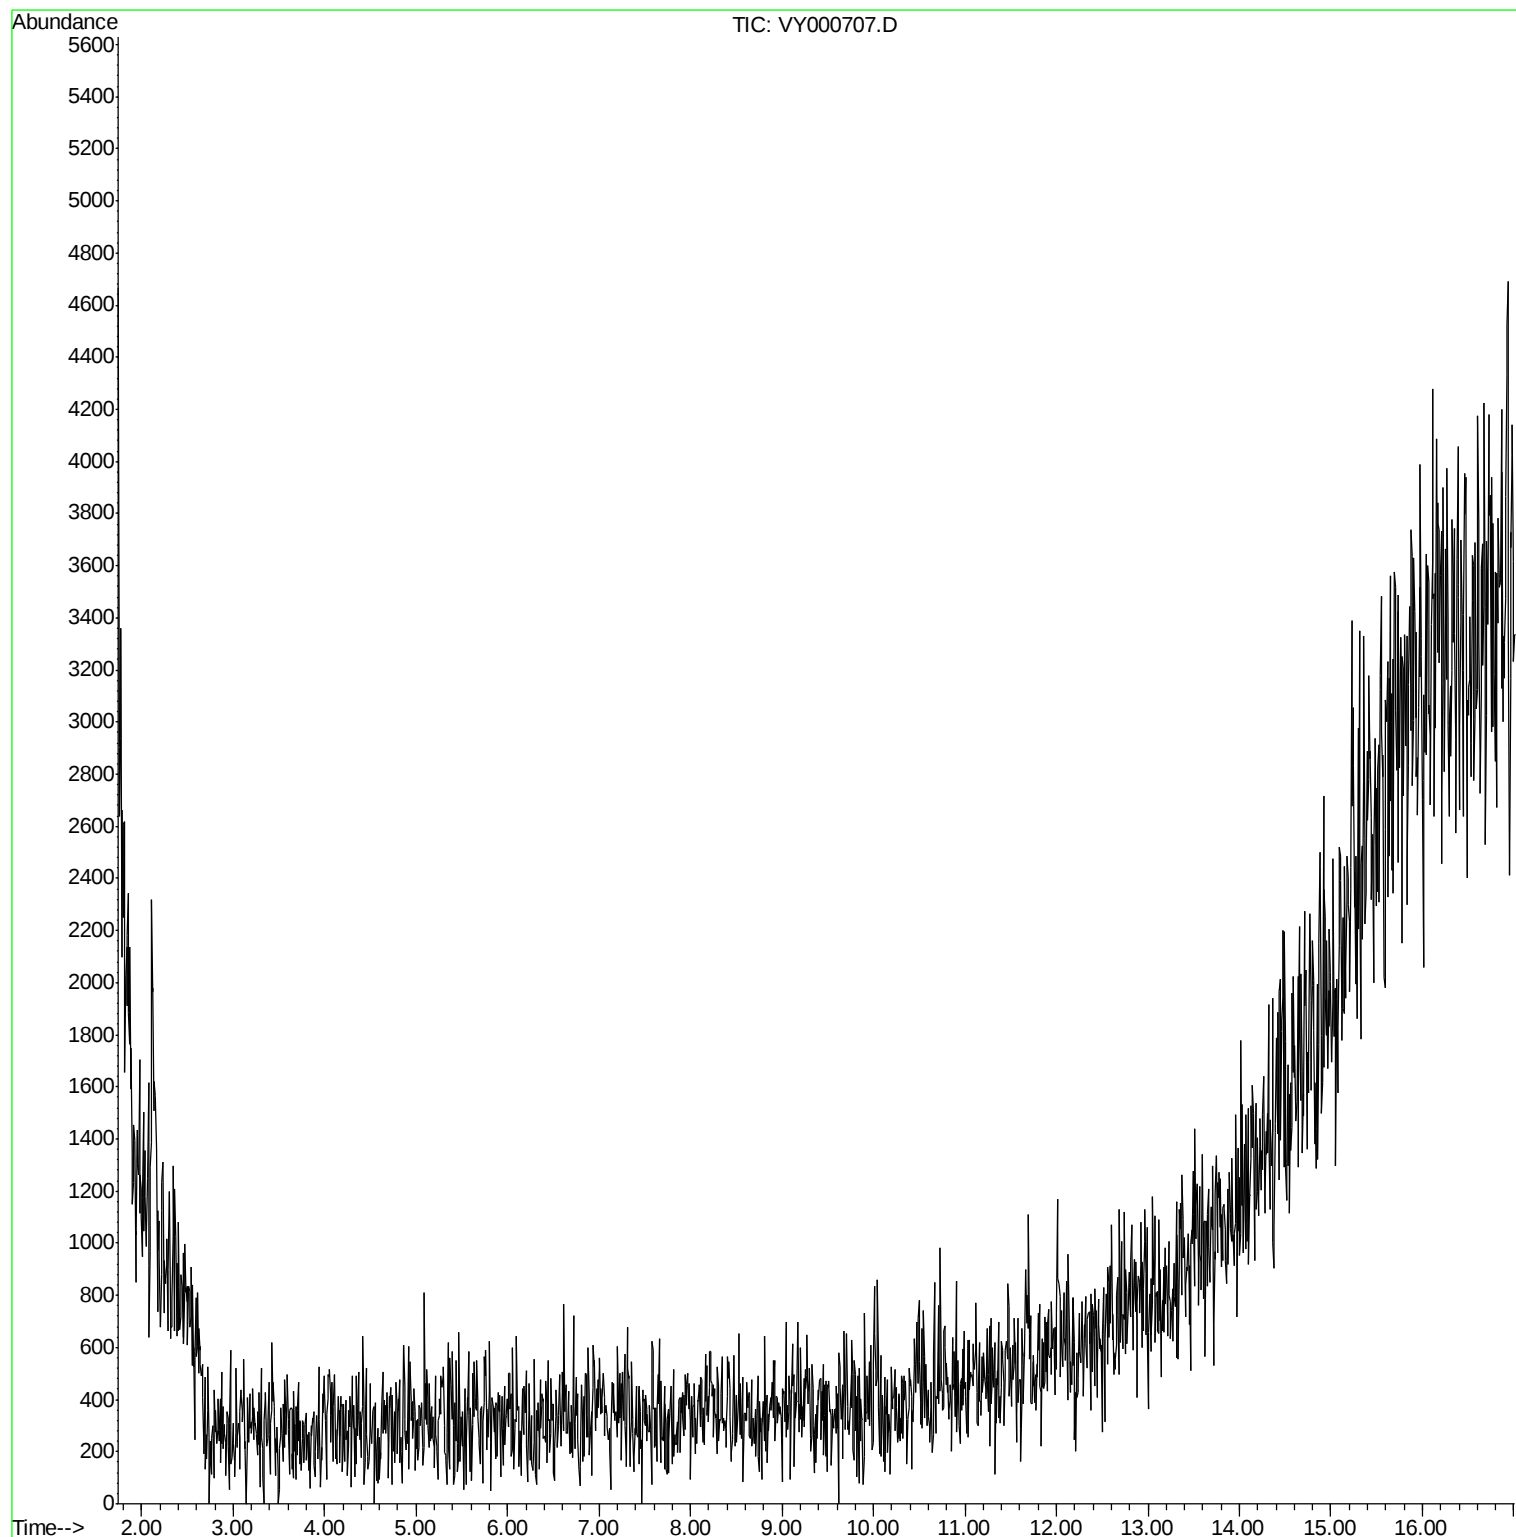

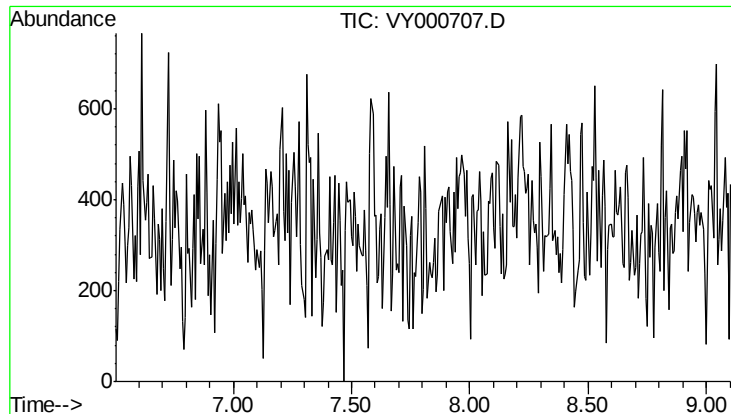

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.80 min

Lab File: VY000707.D

Acq: 15 Nov 2019 17:27

Tgt Ion: 168

Sig Exp Ratio

168 100



99 57.1

Instrument :

MSVOA_Y

ClientSampleId :

EP-15

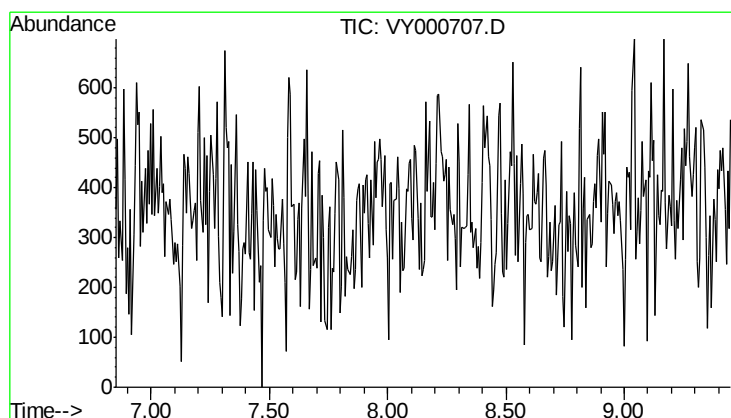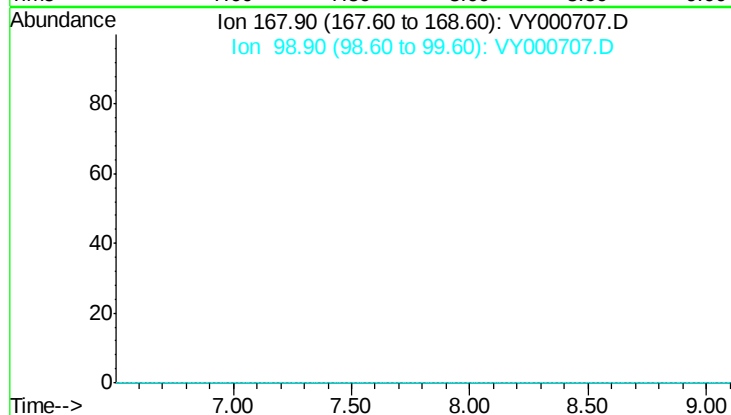

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 8.15 min

Lab File: VY000707.D


Acq: 15 Nov 2019 17:27


Tgt Ion: 65

Sig Exp Ratio

65 100

67 53.6

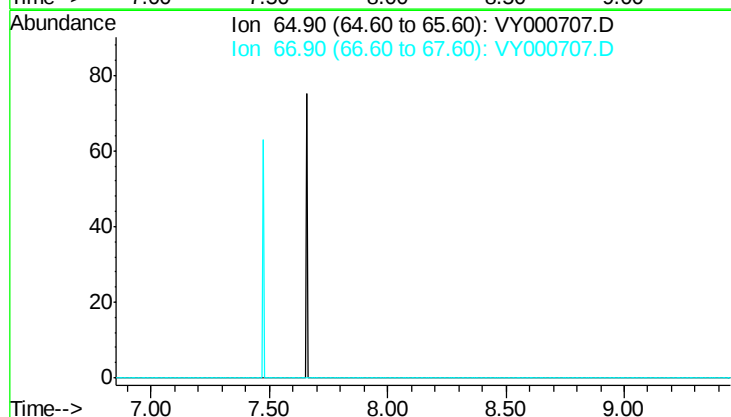


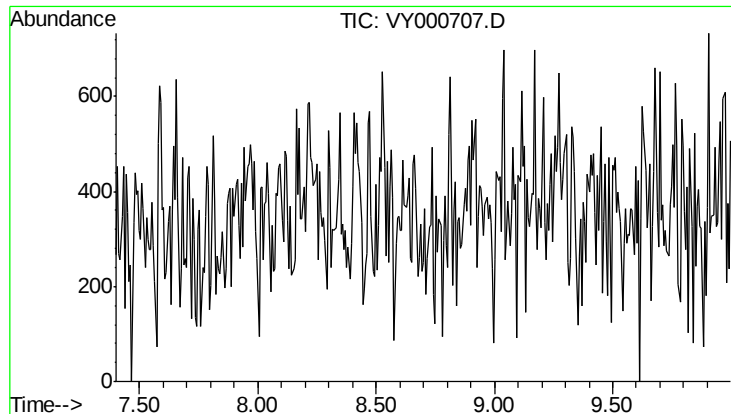


#34
1,4-Difluorobenzene
Concen: 0.000 ug/l
Expected RT: 8.70 min

Lab File: VY000707.D
Acq: 15 Nov 2019 17:27

Instrument :
MSVOA_Y
ClientSampleId :
EP-15


Tgt Ion	114
Sig	Exp Ratio
114	100
63	19.0
88	14.3

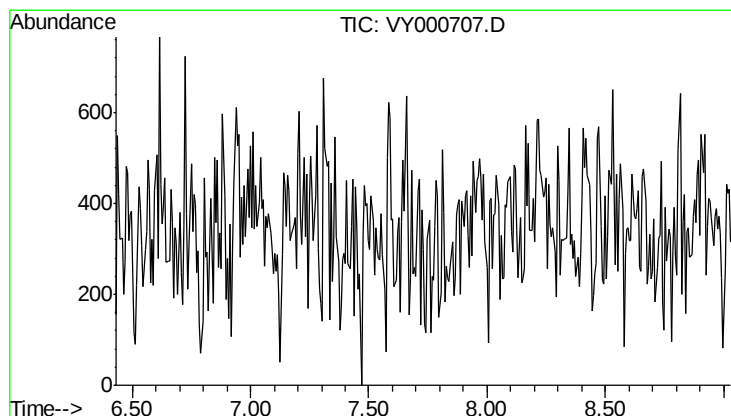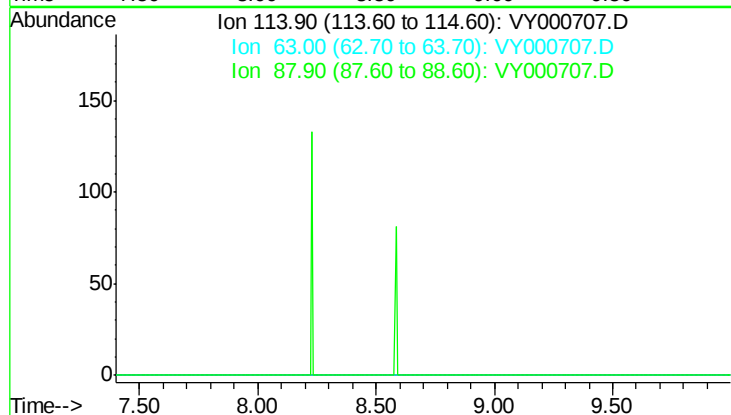


#35
Dibromofluoromethane
Concen: 0.000 ug/l
Expected RT: 7.73 min

Lab File: VY000707.D
Acq: 15 Nov 2019 17:27

Tgt Ion	113
Sig	Exp Ratio
113	100
111	102.1
192	18.7


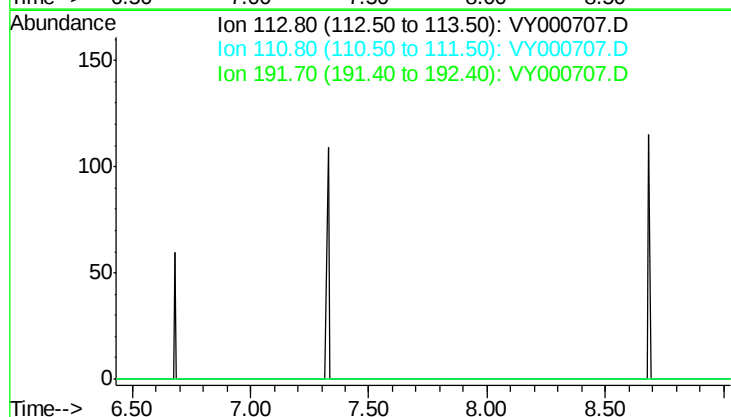


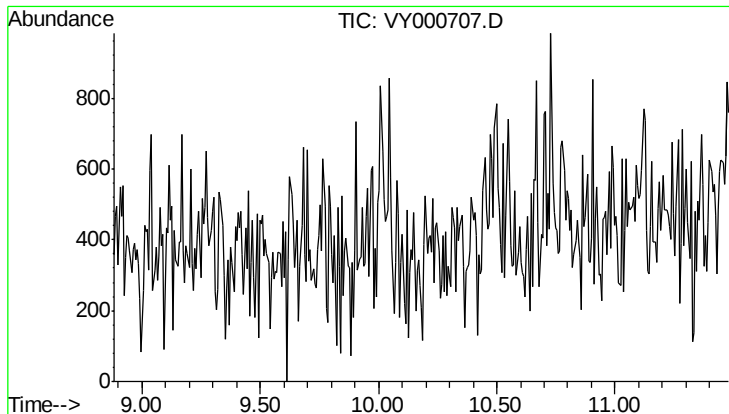

#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.18 min
Lab File: VY000707.D
Acq: 15 Nov 2019 17:27




Instrument :
MSVOA_Y
ClientSampleId :
EP-15


Tgt Ion: 98
Sig Exp Ratio
98 100
100 66.1

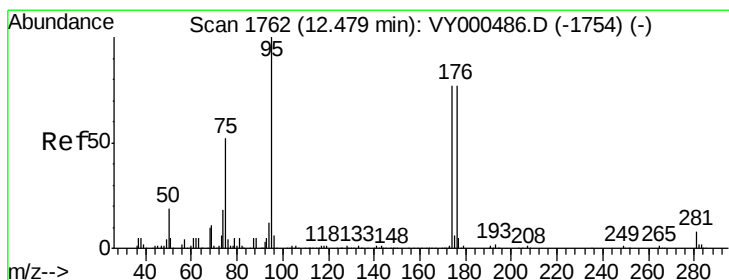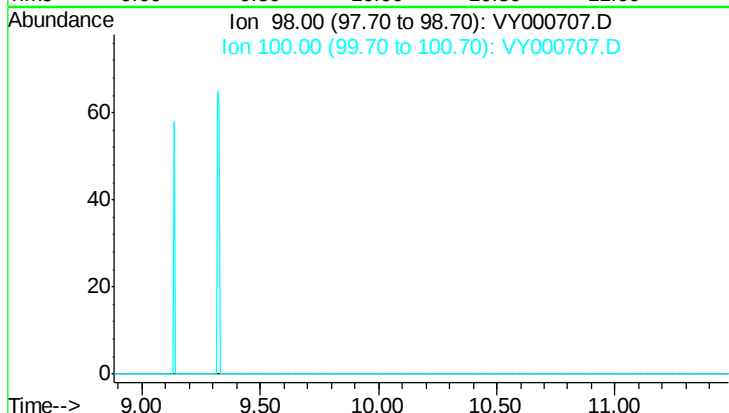

#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
RT: 12.70 min Scan# 1798
Delta R.T. 0.22 min
Lab File: VY000707.D
Acq: 15 Nov 2019 17:27

Tgt Ion: 95 Resp: 46
Ion Ratio Lower Upper
95 100
174 0.0 0.0 161.6
176 0.0 0.0 157.8

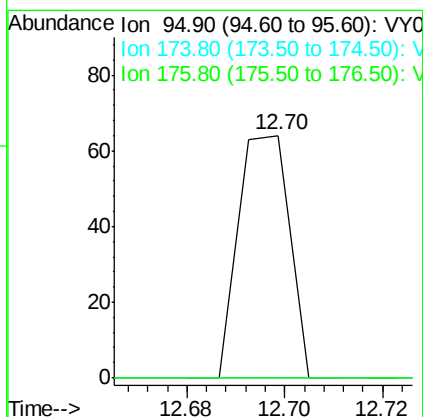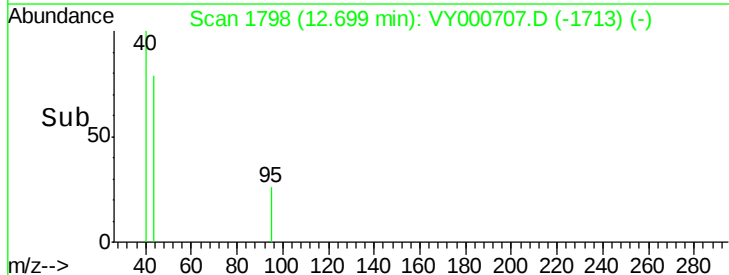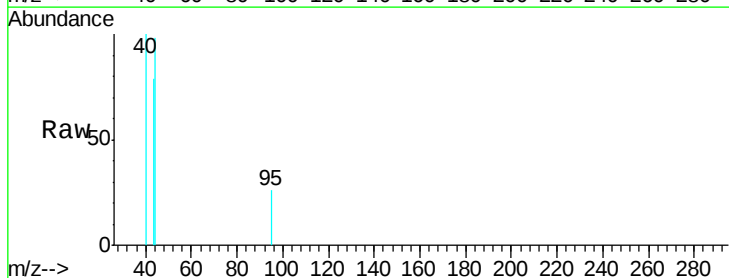


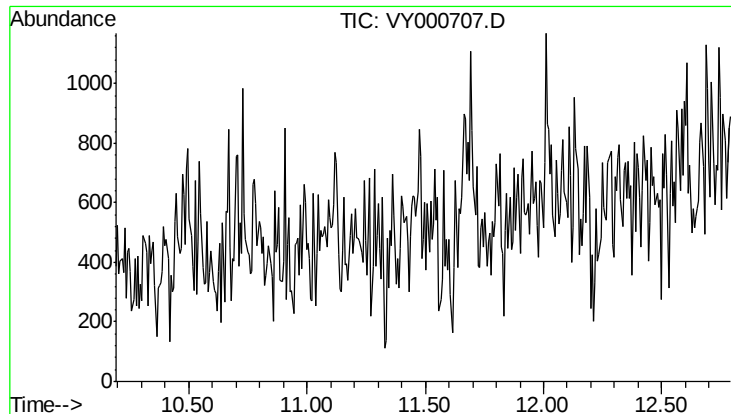


#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.49 min

Lab File: VY000707.D
 Acq: 15 Nov 2019 17:27

Instrument :
 MSVOA_Y
 ClientSampleId :
 EP-15

Tgt Ion: 117
 Sig Exp Ratio
 117 100
 82 51.0
 119 32.7

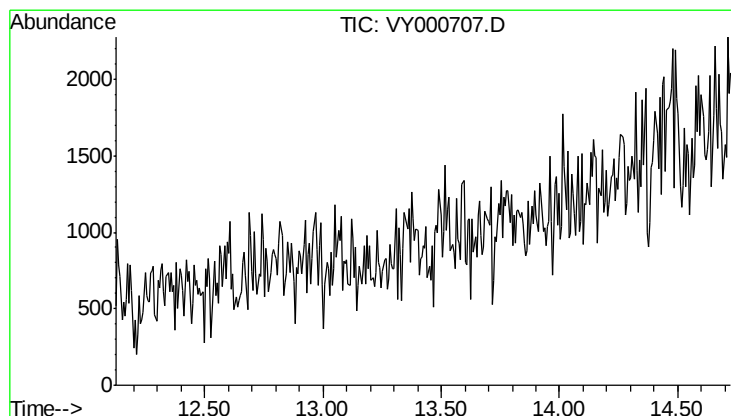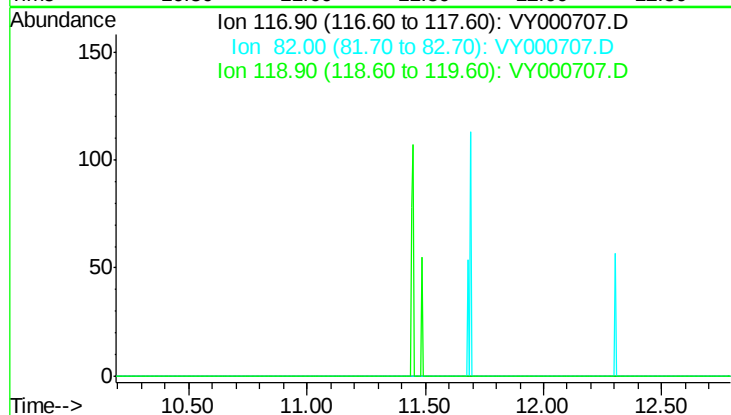

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.42 min

Lab File: VY000707.D
 Acq: 15 Nov 2019 17:27

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 58.3
 150 174.4

