

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_Y\DATA\VY111519\
 Data File : VY000708.D
 Acq On : 15 Nov 2019 17:49
 Operator : SY/MD
 Sample : K5861-19
 Misc : 2.56G/5ML/MSVOA_Y/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 EP-16

Quant Time: Nov 16 02:33:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 30 13:30:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.80
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.70
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.49
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.42

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_Y\DATA\VY111519\
Data File : VY000708.D
Acq On : 15 Nov 2019 17:49
Operator : SY/MD
Sample : K5861-19
Misc : 2.56G/5ML/MSVOA_Y/SOIL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
EP-16

Quant Time: Nov 16 02:33:08 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 30 13:30:53 2019
Response via : Initial Calibration

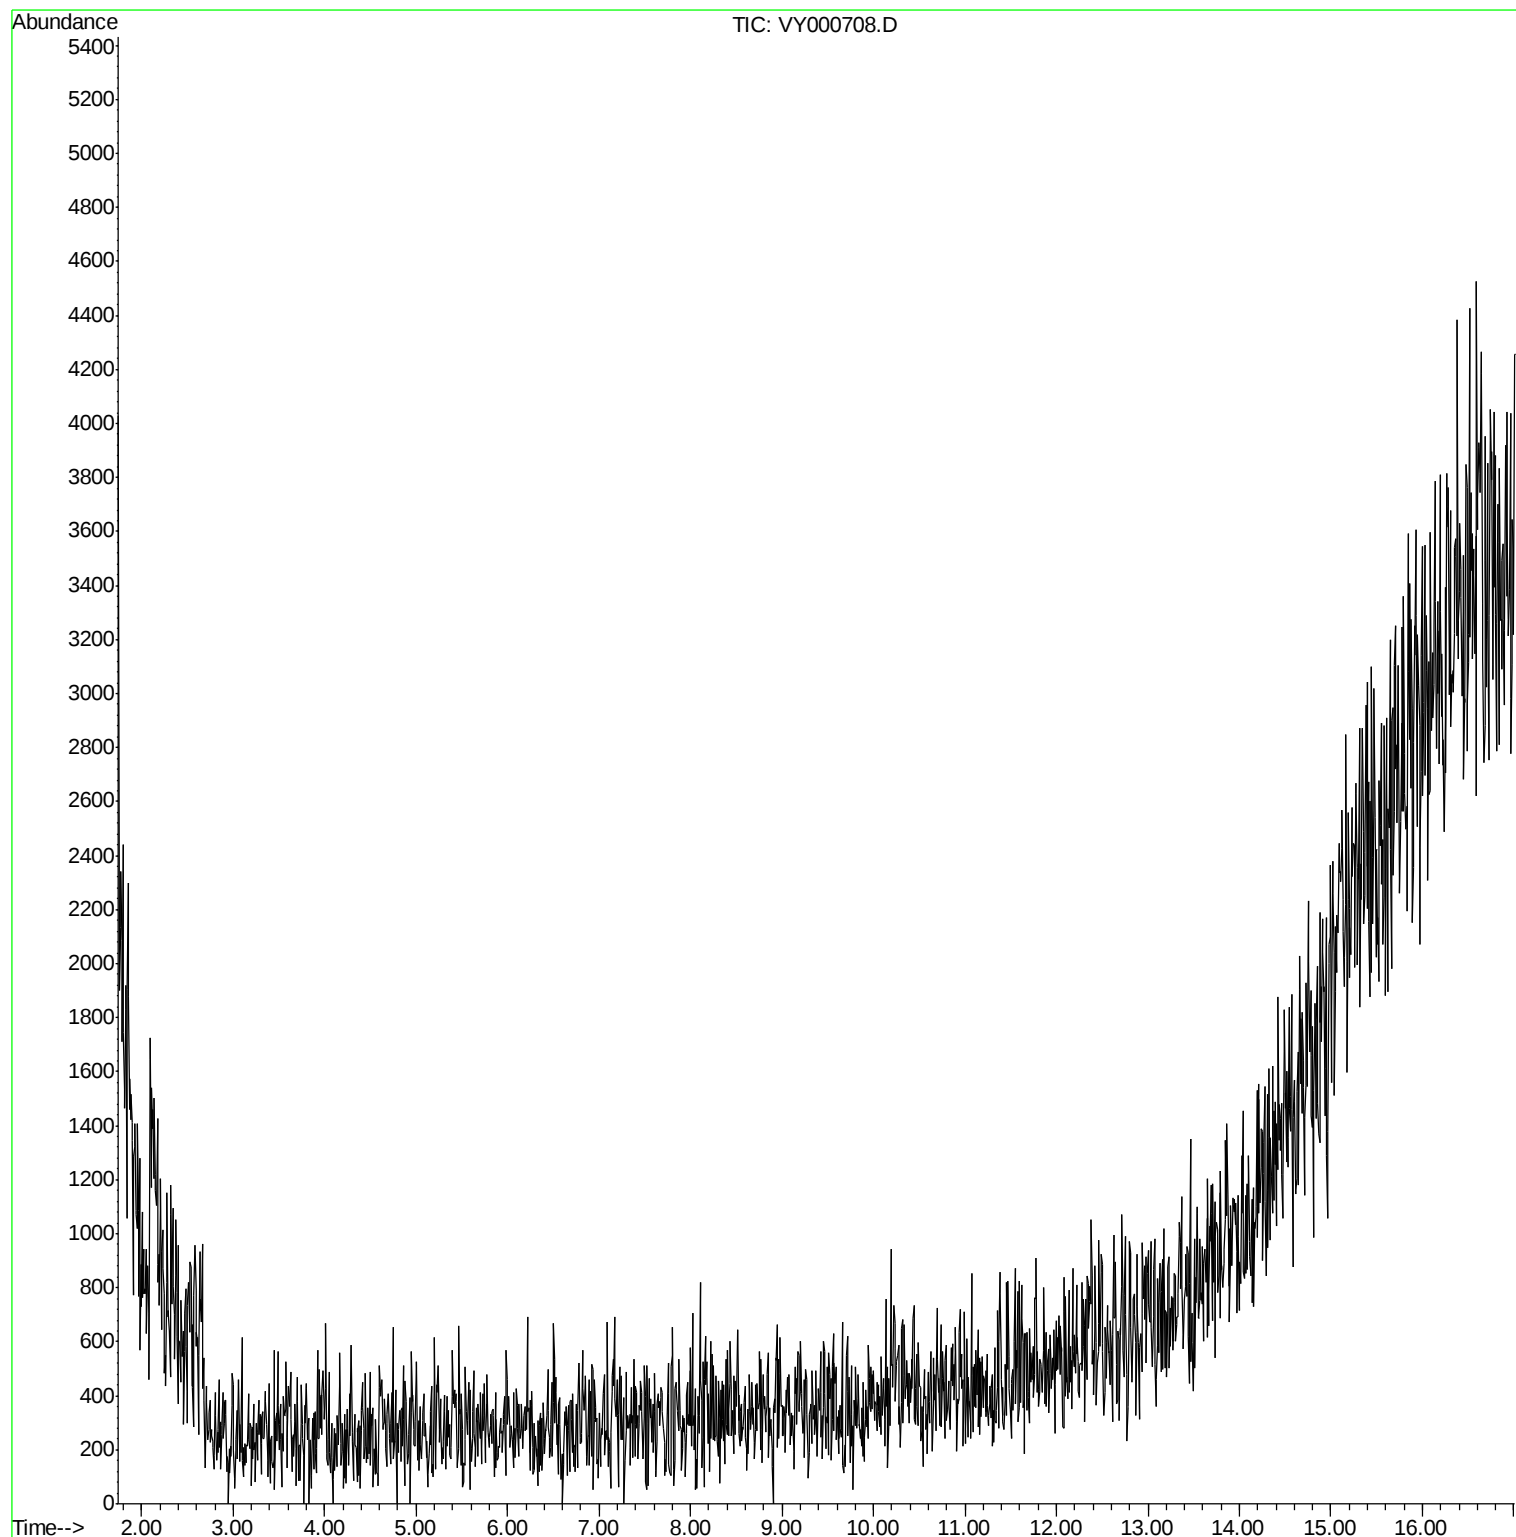

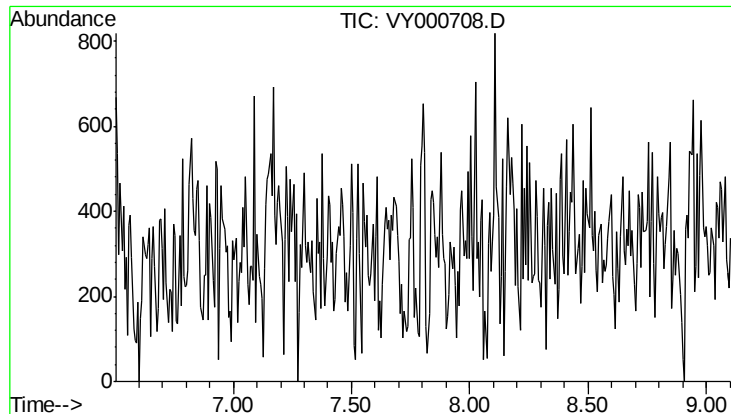

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.80 min

Lab File: VY000708.D

Acq: 15 Nov 2019 17:49

Tgt Ion: 168



Sig	Exp Ratio
168	100
99	57.1

Instrument :

MSVOA_Y

ClientSampleId :

EP-16

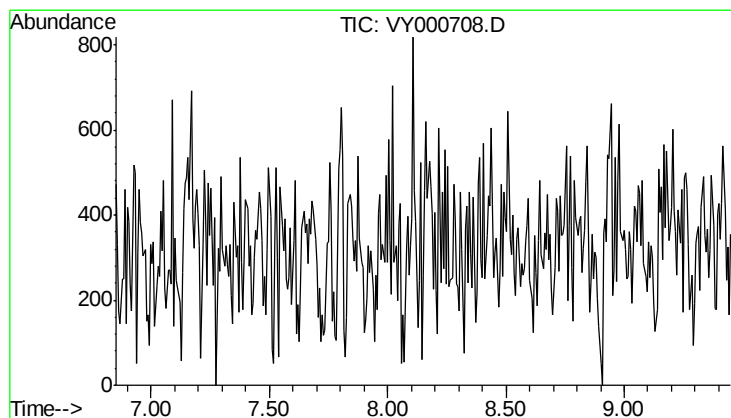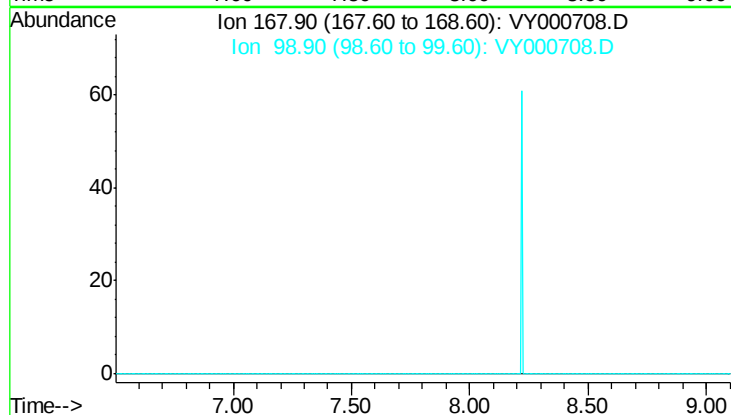

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l


Expected RT: 8.15 min


Lab File: VY000708.D

Acq: 15 Nov 2019 17:49

Tgt Ion: 65

Sig	Exp Ratio
65	100
67	53.6

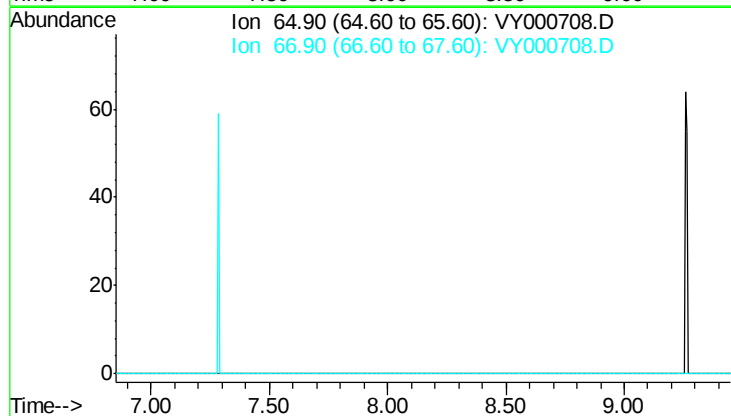

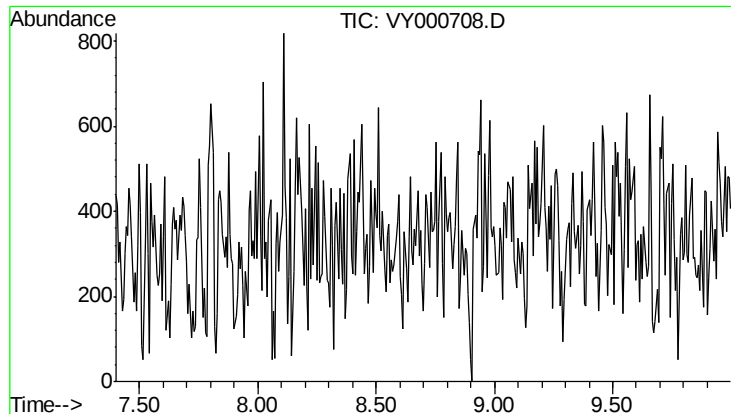

#34

1,4-Difluorobenzene

Concen: 0.000 ug/l

Expected RT: 8.70 min

Lab File: VY000708.D

Acq: 15 Nov 2019 17:49

Instrument :

MSVOA_Y

ClientSampleId :

EP-16



Tgt Ion: 114

Sig Exp Ratio

114 100

63 19.0

88 14.3

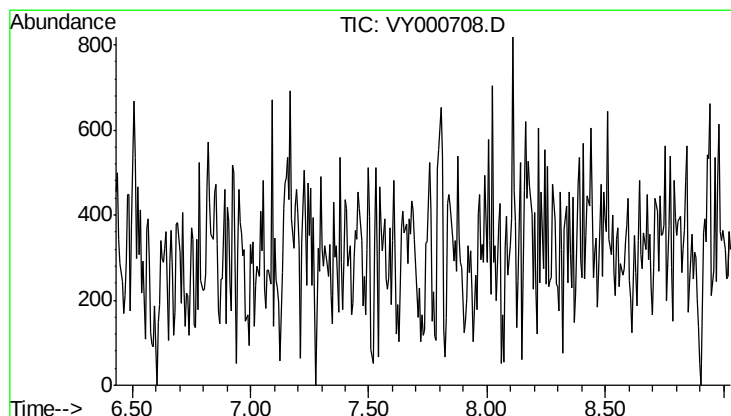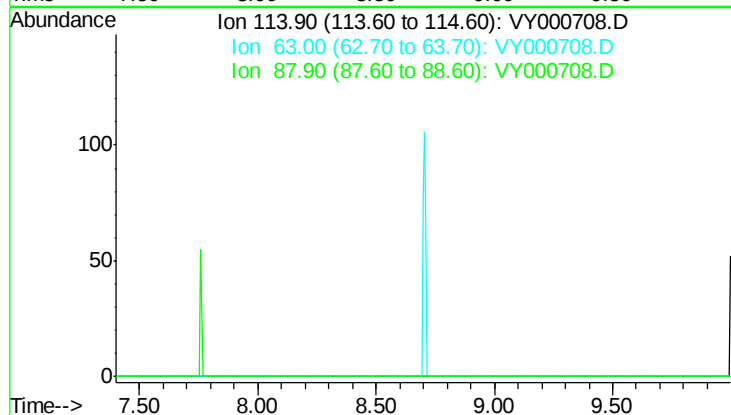

#35

Dibromofluoromethane

Concen: 0.000 ug/l

Expected RT: 7.73 min

Lab File: VY000708.D

Acq: 15 Nov 2019 17:49


Tgt Ion: 113


Sig Exp Ratio

113 100

111 102.1

192 18.7

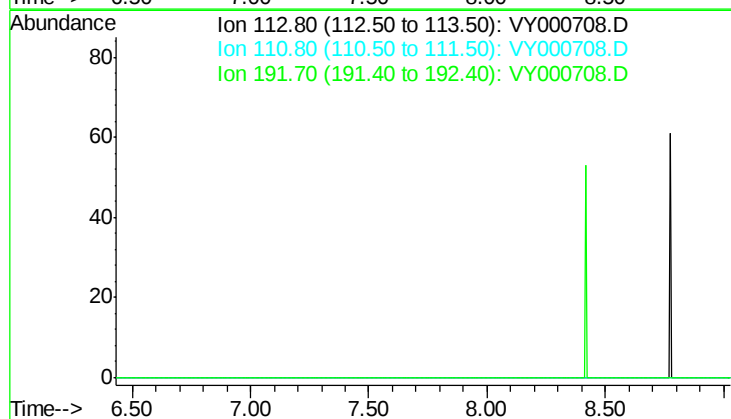


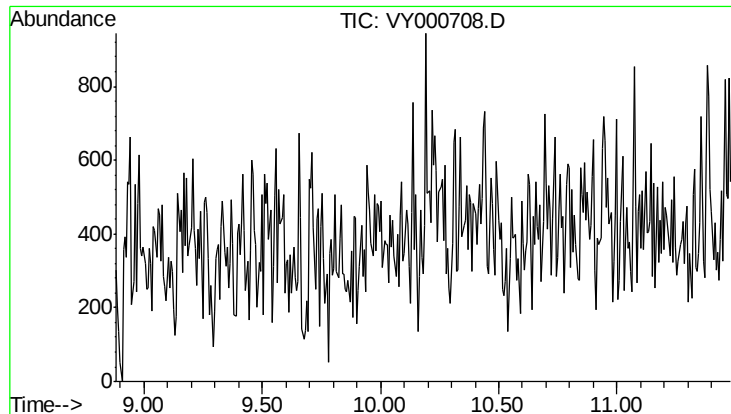


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.18 min

Lab File: VY000708.D
Acq: 15 Nov 2019 17:49

Instrument :
MSVOA_Y
ClientSampleId :
EP-16


Tgt Ion:	98
Sig	Exp Ratio
98	100
100	66.1

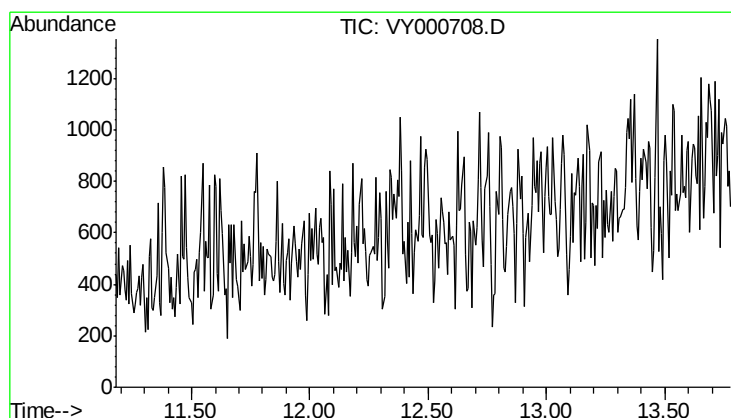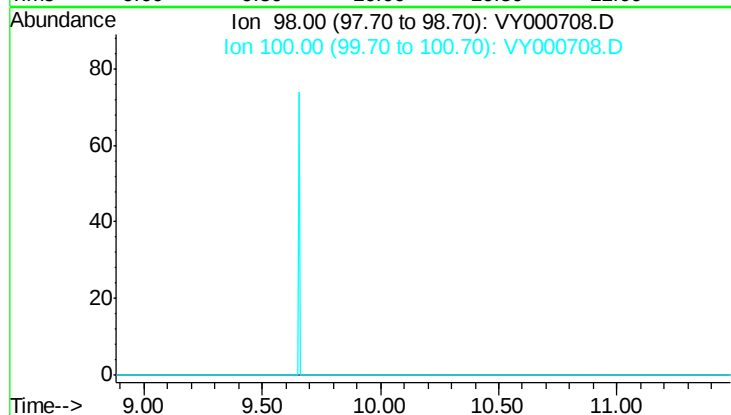


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.48 min

Lab File: VY000708.D
Acq: 15 Nov 2019 17:49

Tgt Ion:	95
Sig	Exp Ratio
95	100
174	80.8
176	78.9

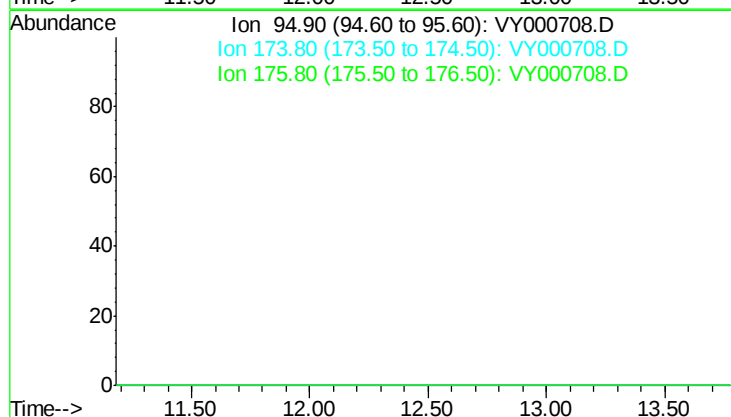


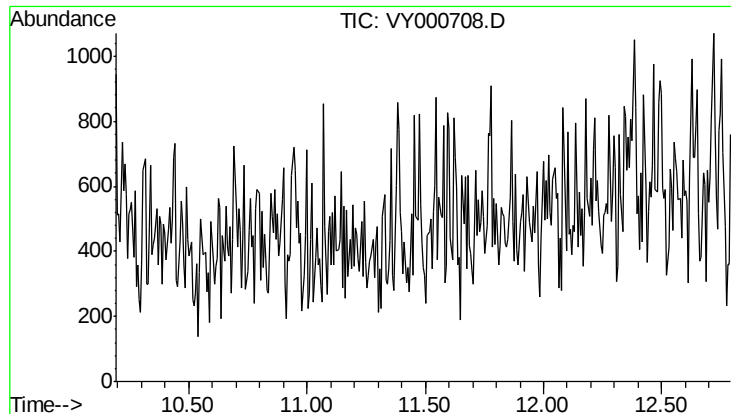


#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.49 min

Lab File: VY000708.D
 Acq: 15 Nov 2019 17:49

Instrument :
 MSVOA_Y
 ClientSampleId :
 EP-16

Tgt Ion: 117
 Sig Exp Ratio
 117 100
 82 51.0
 119 32.7

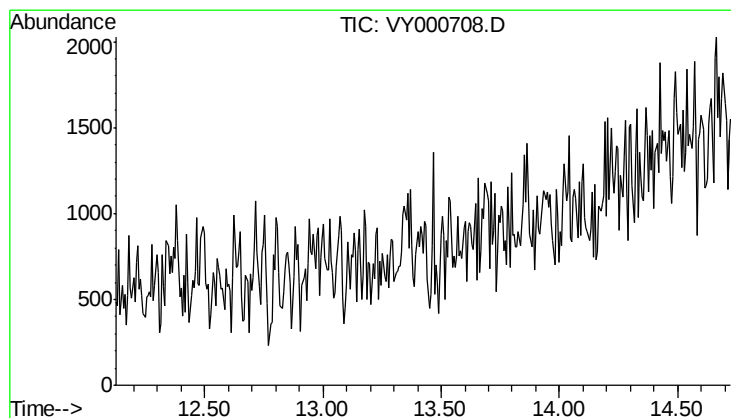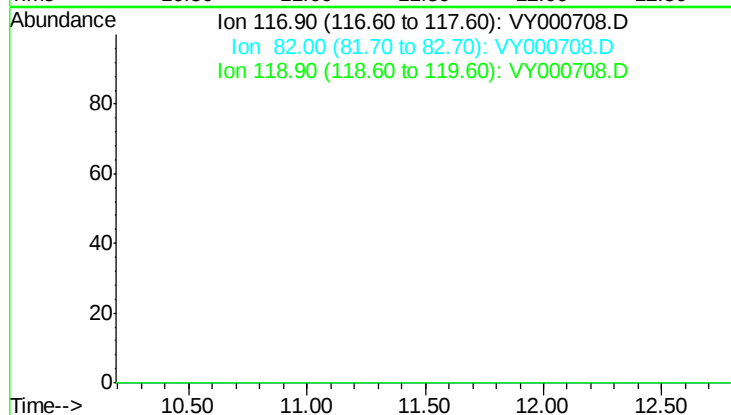

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.42 min

Lab File: VY000708.D
 Acq: 15 Nov 2019 17:49

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 58.3
 150 174.4

