

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY111622\
 Data File : VY011474.D
 Acq On : 16 Nov 2022 15:31
 Operator : KP/MD
 Sample : N5641-04
 Misc : 6.72g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Nov 17 03:16:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111022S.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 10 17:47:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	334216	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	552307	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	476137	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	198687	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	165809	59.204	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 118.400%	
35) Dibromofluoromethane	7.716	113	182961	59.110	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 118.220%	
50) Toluene-d8	10.179	98	667200	56.424	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 112.840%	
62) 4-Bromofluorobenzene	12.483	95	208932	50.658	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 101.320%	
Target Compounds						Qvalue
11) Tert butyl alcohol	4.912	59	367	Below Cal	#	77
16) Acetone	3.948	43	892	1.207	ug/l	98
18) Methyl Acetate	4.485	43	147	Below Cal	#	56
20) Methylene Chloride	4.716	84	21405	Below Cal	#	72
31) Cyclohexane	7.789	56	5294	1.052	ug/l	# 1
36) 1,1-Dichloropropene	7.789	75	22261	4.634	ug/l	# 51
38) Carbon Tetrachloride	7.789	117	31440	6.016	ug/l	# 16
76) 1,2,3-Trichloropropane	12.483	75	98697	42.914	ug/l	# 100
81) trans-1,4-Dichloro-2-b...	12.483	75	98697	103.153	ug/l	# 7
95) Naphthalene	15.245	128	454	3.332	ug/l	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY111622\
Data File : VY011474.D
Acq On : 16 Nov 2022 15:31
Operator : KP/MD
Sample : N5641-04
Misc : 6.72g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :

Quant Time: Nov 17 03:16:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111022S.M
Quant Title : SW846 8260
QLast Update : Thu Nov 10 17:47:26 2022
Response via : Initial Calibration




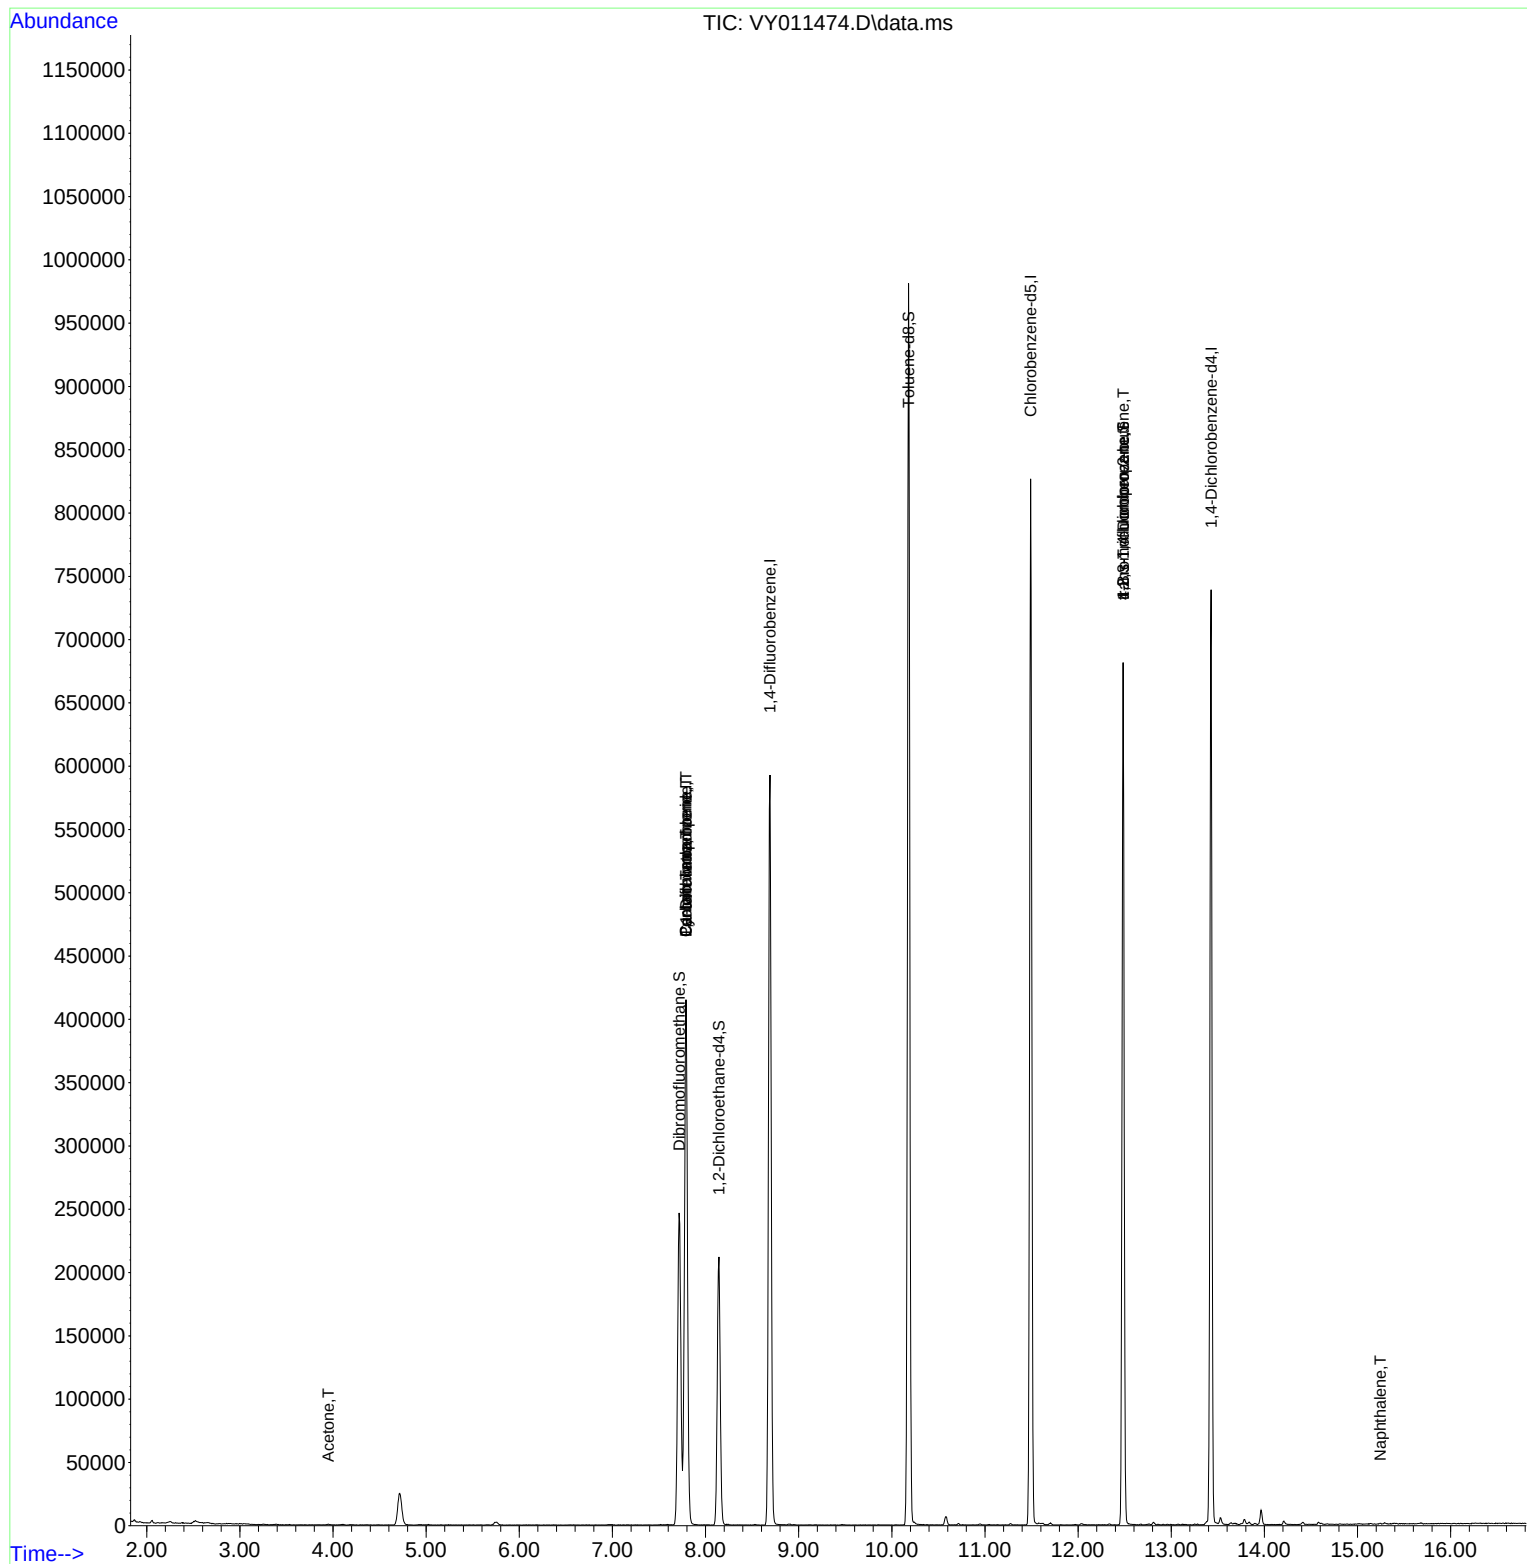


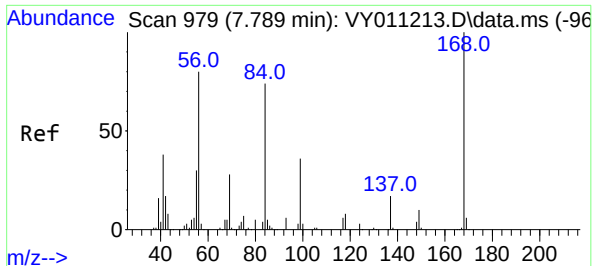

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY011474.D
Acq: 16 Nov 2022 15:31




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:168 Resp: 334216
Ion Ratio Lower Upper
168 100
99 52.3 46.9 70.3

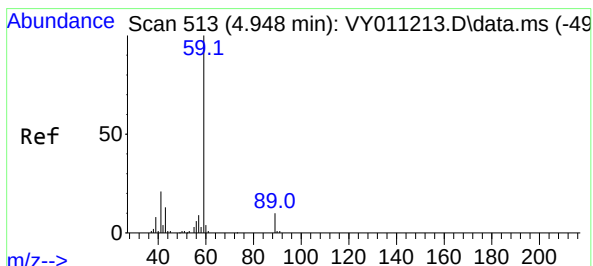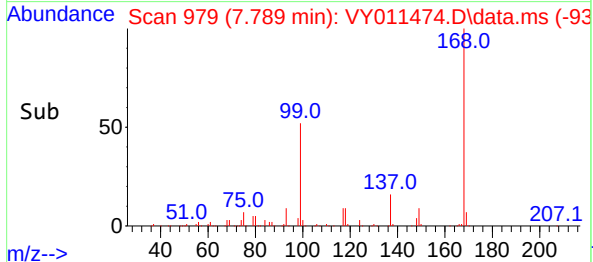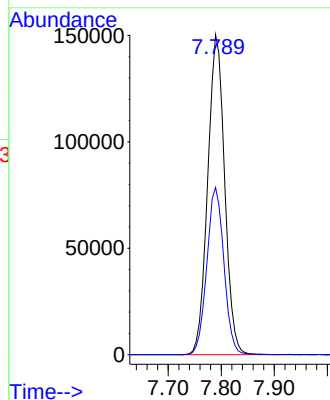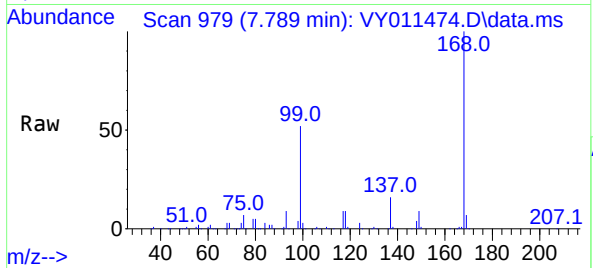

#11
Tert butyl alcohol
Concen: Below Cal
RT: 4.912 min Scan# 507
Delta R.T. -0.042 min
Lab File: VY011474.D
Acq: 16 Nov 2022 15:31

Tgt Ion: 59 Resp: 367
Ion Ratio Lower Upper
59 100
57 0.0 6.4 9.6#


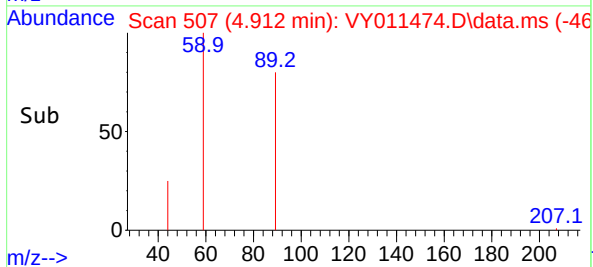
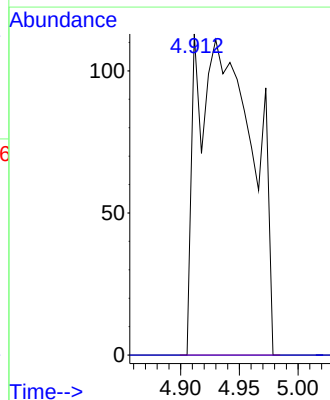
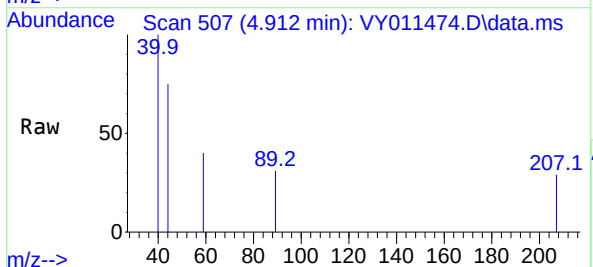




#16
Acetone
Concen: 1.207 ug/l
RT: 3.948 min Scan# 348
Delta R.T. 0.006 min
Lab File: VY011474.D
Acq: 16 Nov 2022 15:31




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 43 Resp: 892
Ion Ratio Lower Upper
43 100
58 26.7 22.0 33.0

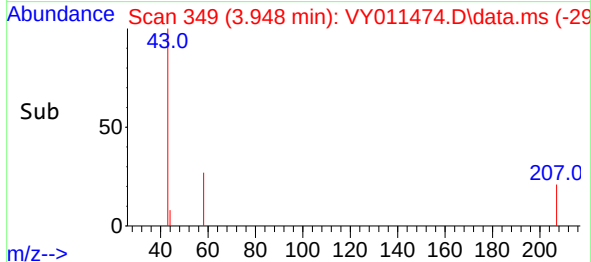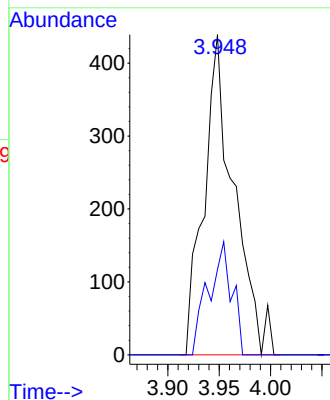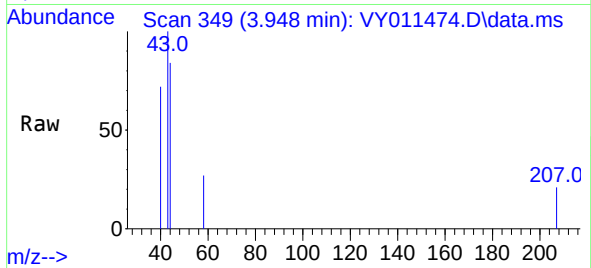

#18
Methyl Acetate
Concen: Below Cal
RT: 4.485 min Scan# 437
Delta R.T. 0.012 min
Lab File: VY011474.D
Acq: 16 Nov 2022 15:31


Tgt Ion: 43 Resp: 147
Ion Ratio Lower Upper
43 100
74 0.0 16.6 24.8#

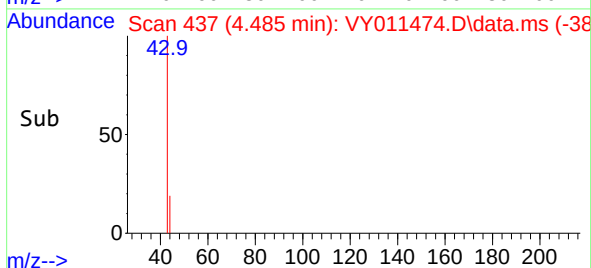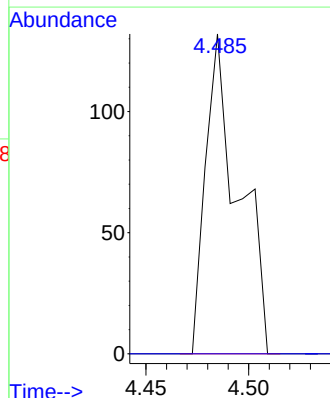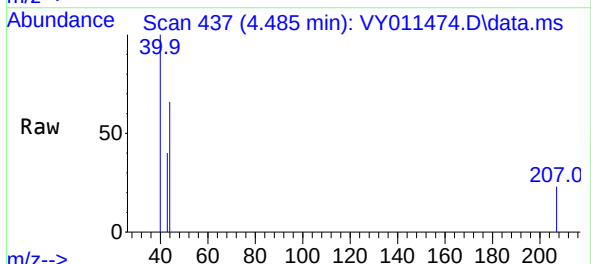






#20
Methylene Chloride
Concen: Below Cal
RT: 4.716 min Scan# 41
Delta R.T. 0.006 min
Lab File: VY011474.D
Acq: 16 Nov 2022 15:31

Instrument :
MSVOA_Y
ClientSampleId :

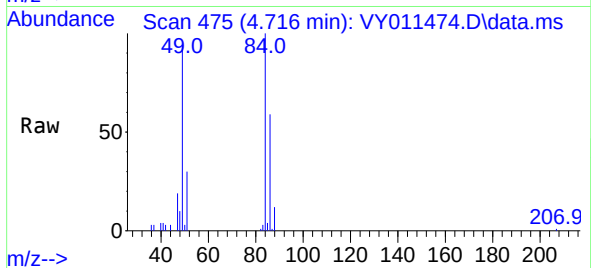

Tgt Ion: 84 Resp: 21405




Ion	Ratio	Lower	Upper
84	100		
49	94.5	114.4	171.6#
51	30.2	35.3	52.9#
86	59.4	53.7	80.5

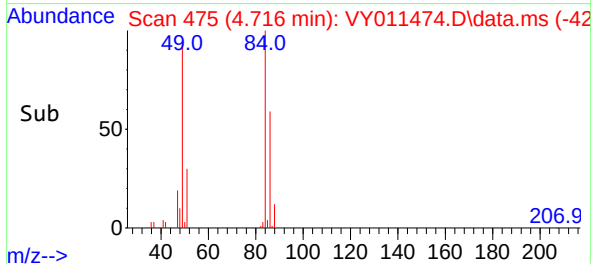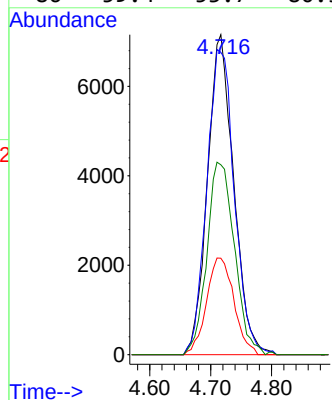


#31
Cyclohexane
Concen: 1.052 ug/l
RT: 7.789 min Scan# 979
Delta R.T. 0.006 min
Lab File: VY011474.D
Acq: 16 Nov 2022 15:31

Tgt Ion: 56 Resp: 5294

Ion	Ratio	Lower	Upper
56	100		
69	212.1	26.7	40.1#
84	193.9	67.2	100.8#

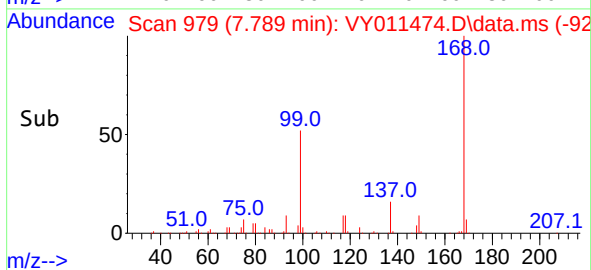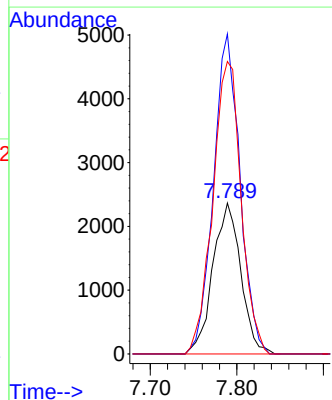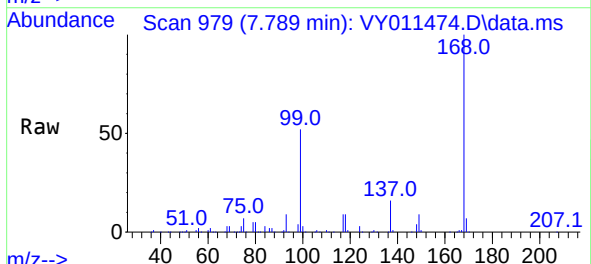

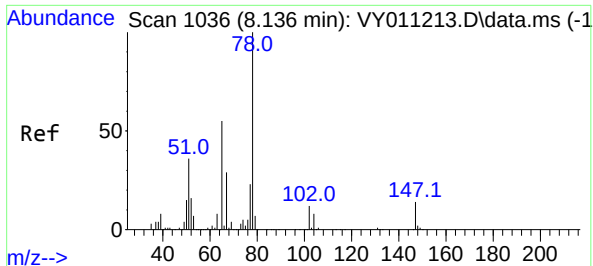

#33

1,2-Dichloroethane-d4

Concen: 59.204 ug/l

RT: 8.143 min Scan# 1

Delta R.T. 0.007 min

Lab File: VY011474.D

Acq: 16 Nov 2022 15:31

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion: 65 Resp: 165809

Ion Ratio Lower Upper

65 100

67 54.0 0.0 99.4

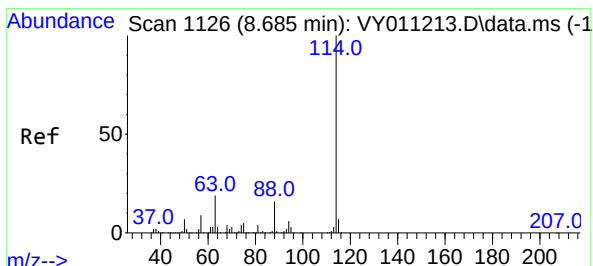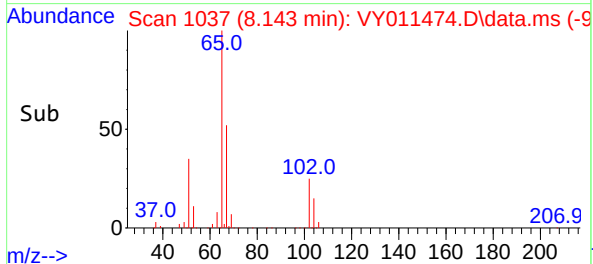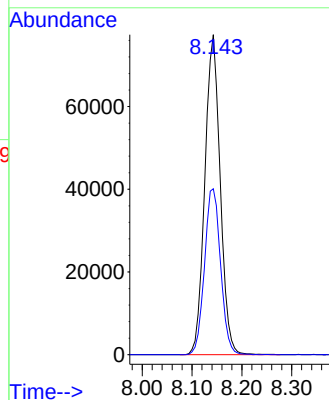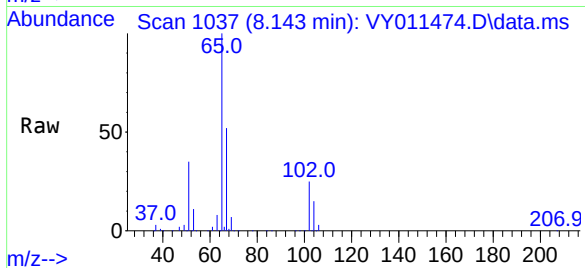

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY011474.D

Acq: 16 Nov 2022 15:31




Tgt Ion:114 Resp: 552307


Ion Ratio Lower Upper

114 100

63 17.6 0.0 43.2

88 15.1 0.0 31.8


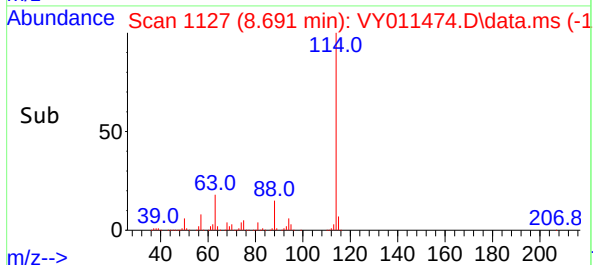
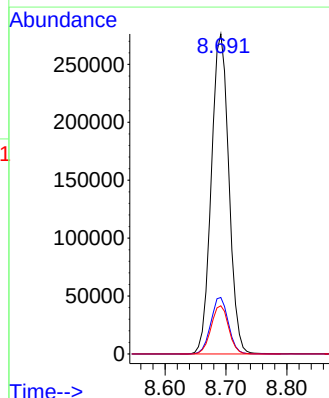
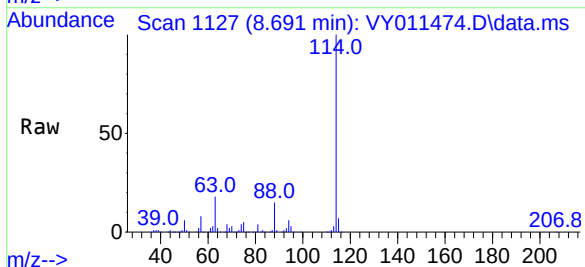




#35
Dibromofluoromethane
Concen: 59.110 ug/l
RT: 7.716 min Scan# 901
Delta R.T. 0.006 min
Lab File: VY011474.D
Acq: 16 Nov 2022 15:31




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:113 Resp: 182961
Ion Ratio Lower Upper
113 100
111 101.7 82.6 124.0
192 20.7 17.6 26.4

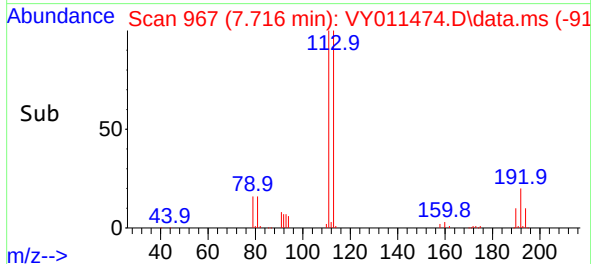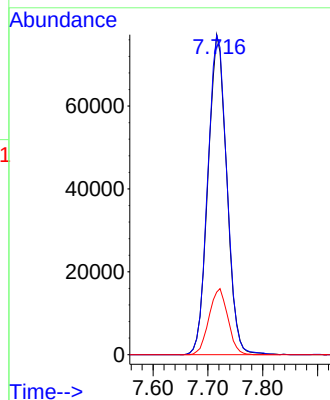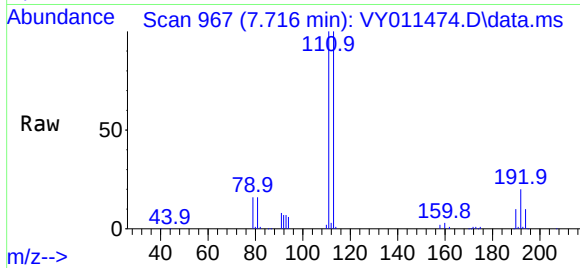

#36
1,1-Dichloropropene
Concen: 4.634 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.128 min
Lab File: VY011474.D
Acq: 16 Nov 2022 15:31


Tgt Ion: 75 Resp: 22261
Ion Ratio Lower Upper
75 100
110 9.3 17.1 51.2#
77 0.0 24.4 36.6#

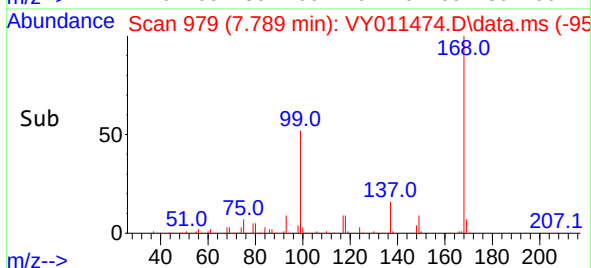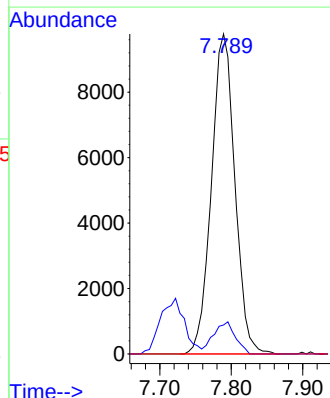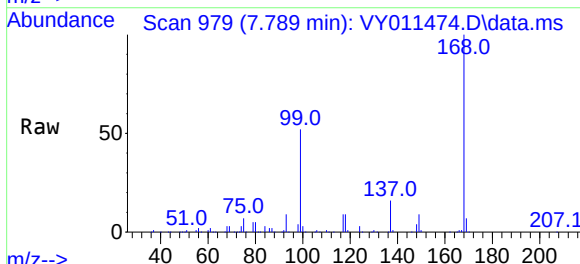






#38
Carbon Tetrachloride
Concen: 6.016 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.110 min
Lab File: VY011474.D
Acq: 16 Nov 2022 15:31

Instrument :
MSVOA_Y
ClientSampleId :



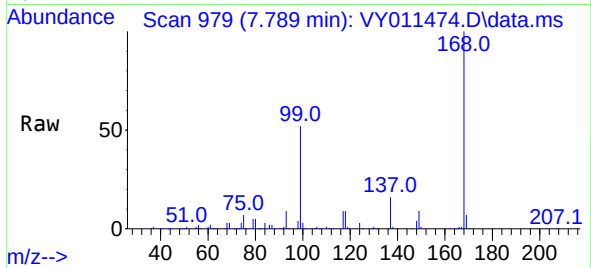



Tgt Ion:117 Resp: 31440
Ion Ratio Lower Upper
117 100
119 5.5 77.9 116.9#
121 0.0 24.8 37.2#

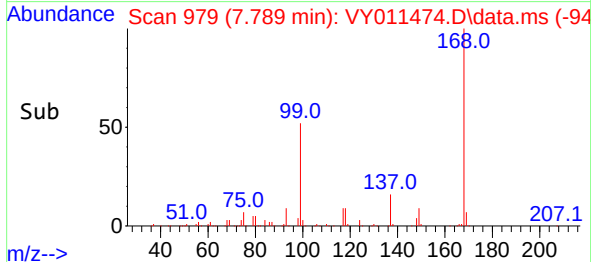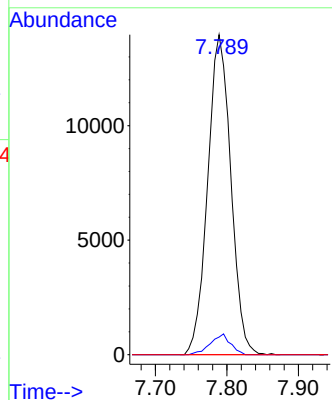

#50
Toluene-d8
Concen: 56.424 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY011474.D
Acq: 16 Nov 2022 15:31

Tgt Ion: 98 Resp: 667200
Ion Ratio Lower Upper
98 100
100 65.4 50.2 75.2


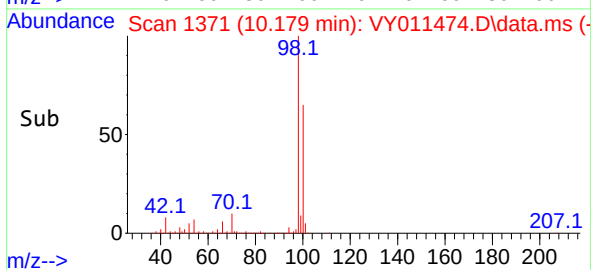
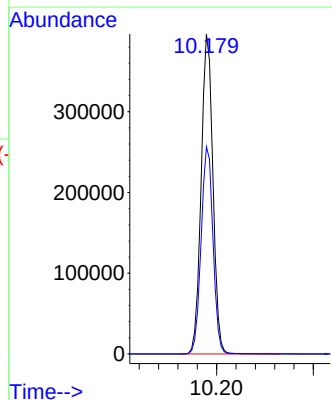
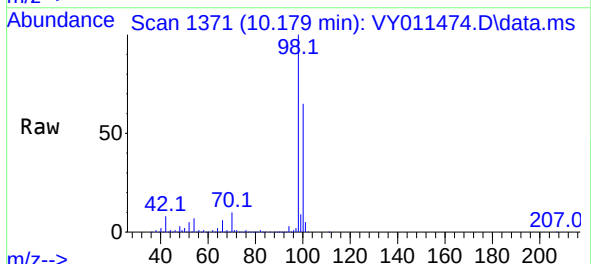


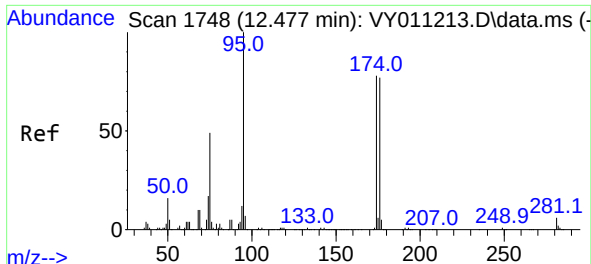

#62
4-Bromofluorobenzene
Concen: 50.658 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY011474.D
Acq: 16 Nov 2022 15:31




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 95 Resp: 208932
Ion Ratio Lower Upper
95 100
174 88.4 0.0 177.0
176 85.5 0.0 175.8

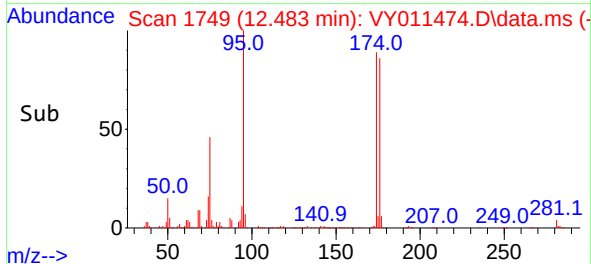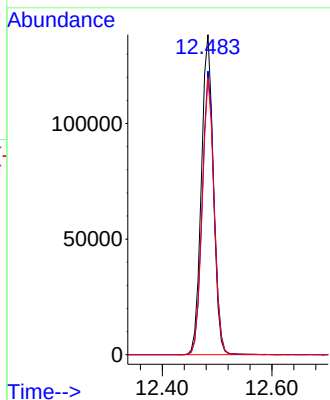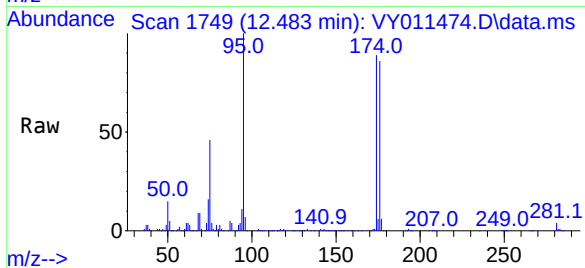

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. -0.000 min
Lab File: VY011474.D
Acq: 16 Nov 2022 15:31

Tgt Ion: 117 Resp: 476137
Ion Ratio Lower Upper
117 100
82 53.2 43.0 64.4
119 31.8 25.4 38.0


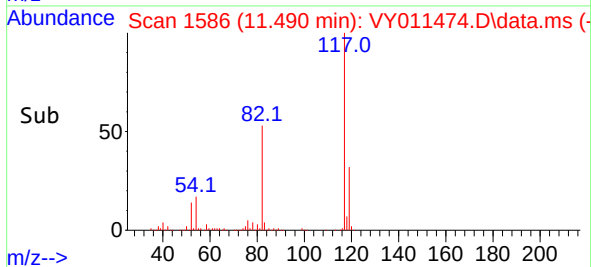
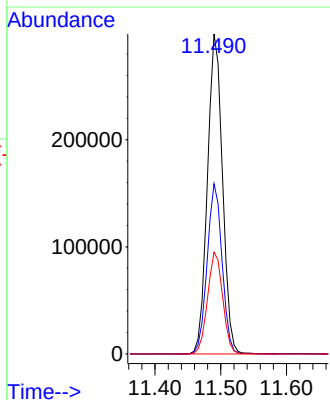
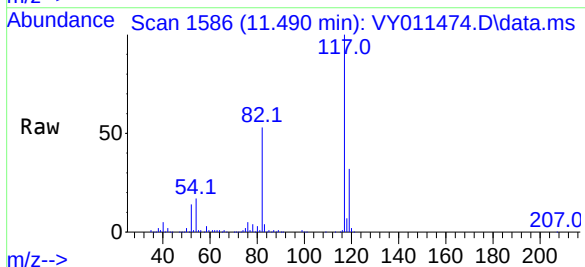




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.428 min Scan# 1903
 Delta R.T. 0.006 min
 Lab File: VY011474.D
 Acq: 16 Nov 2022 15:31




Instrument :
 MSVOA_Y
 ClientSampleId :


Tgt Ion:152 Resp: 198687
 Ion Ratio Lower Upper
 152 100
 115 57.0 28.2 84.7
 150 157.9 0.0 347.6

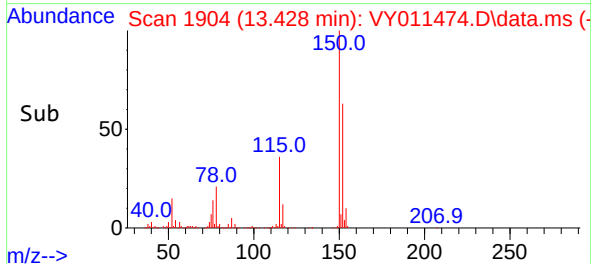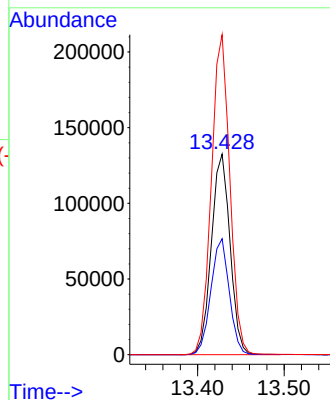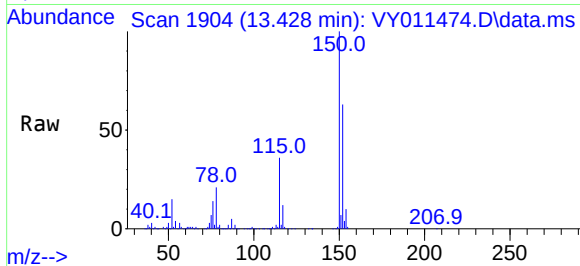

#76
 1,2,3-Trichloropropane
 Concen: 42.914 ug/l
 RT: 12.483 min Scan# 1749
 Delta R.T. -0.147 min
 Lab File: VY011474.D
 Acq: 16 Nov 2022 15:31


Tgt Ion: 75 Resp: 98697
 Ion Ratio Lower Upper
 75 100
 77 1.3 0.0 0.0#

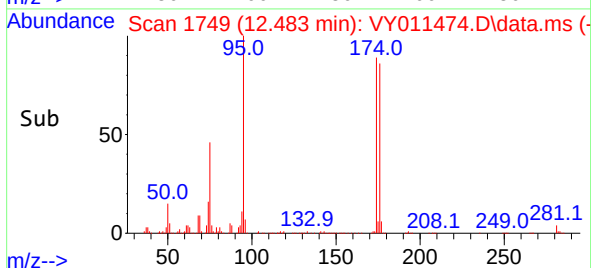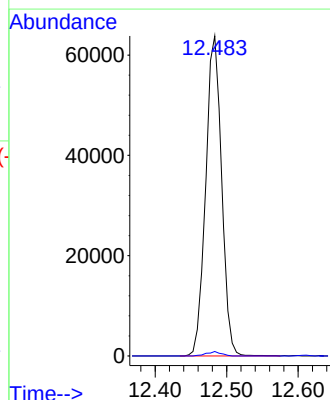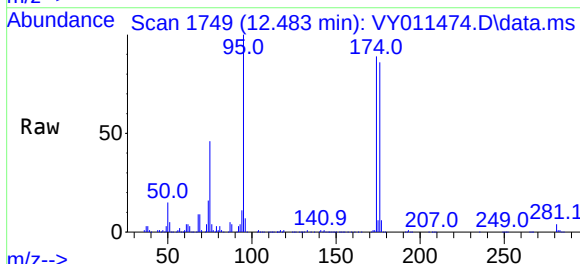






#81
trans-1,4-Dichloro-2-butene
Concen: 103.153 ug/l
RT: 12.483 min Scan# 11
Delta R.T. 0.103 min
Lab File: VY011474.D
Acq: 16 Nov 2022 15:31

Instrument :
MSVOA_Y
ClientSampleId :

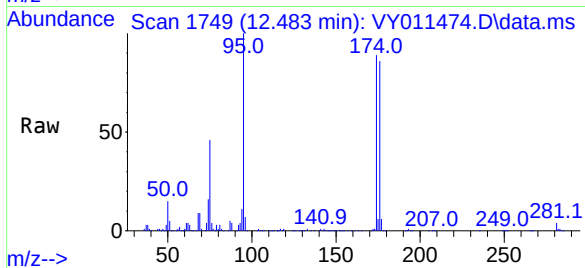

Tgt Ion: 75 Resp: 98697
Ion Ratio Lower Upper
75 100
53 0.1 85.3 127.9#
89 0.0 37.0 55.4#

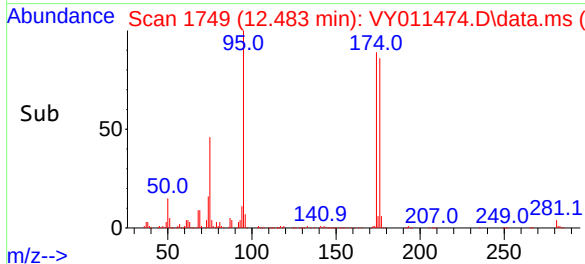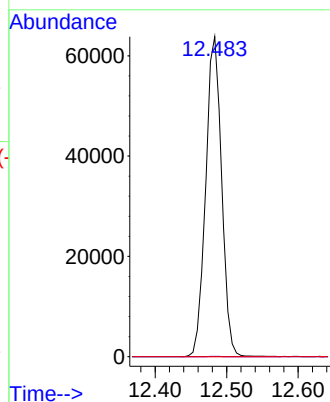

#95
Naphthalene
Concen: 3.332 ug/l
RT: 15.245 min Scan# 2202
Delta R.T. 0.012 min
Lab File: VY011474.D
Acq: 16 Nov 2022 15:31

Tgt Ion: 128 Resp: 454
Ion Ratio Lower Upper
128 100
127 0.0 11.0 16.4#
129 0.0 8.4 12.6#

