
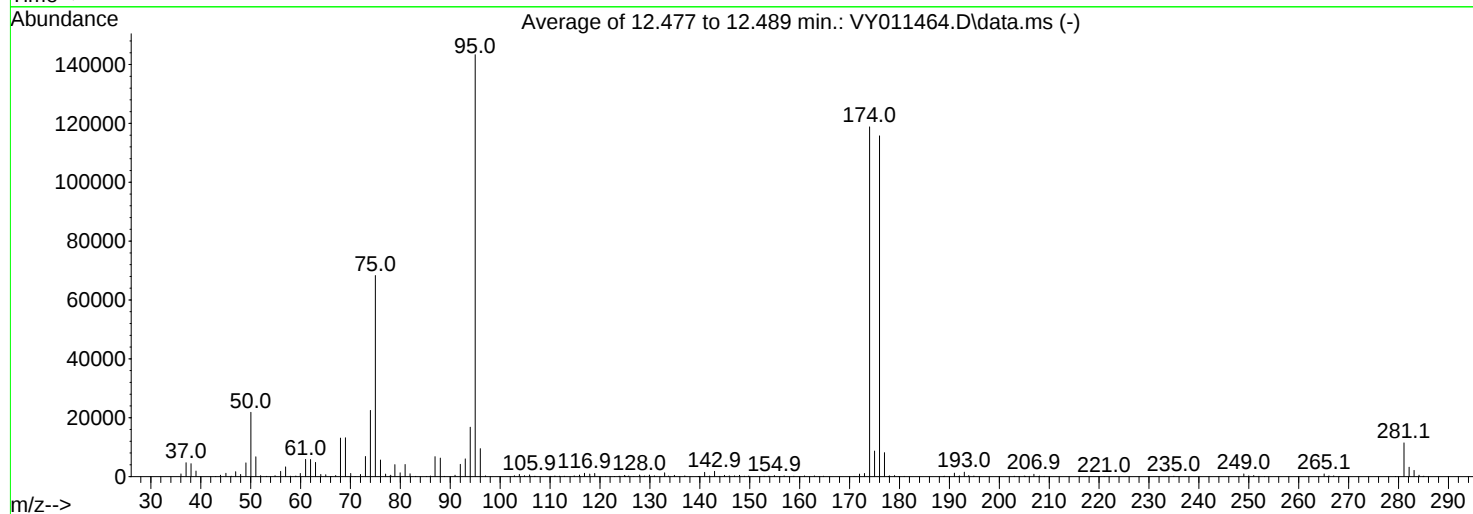


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY111622\
 Data File : VY011464.D
 Acq On : 16 Nov 2022 10:13
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111022S.M
 Title : SW846 8260
 Last Update : Thu Nov 10 17:47:26 2022

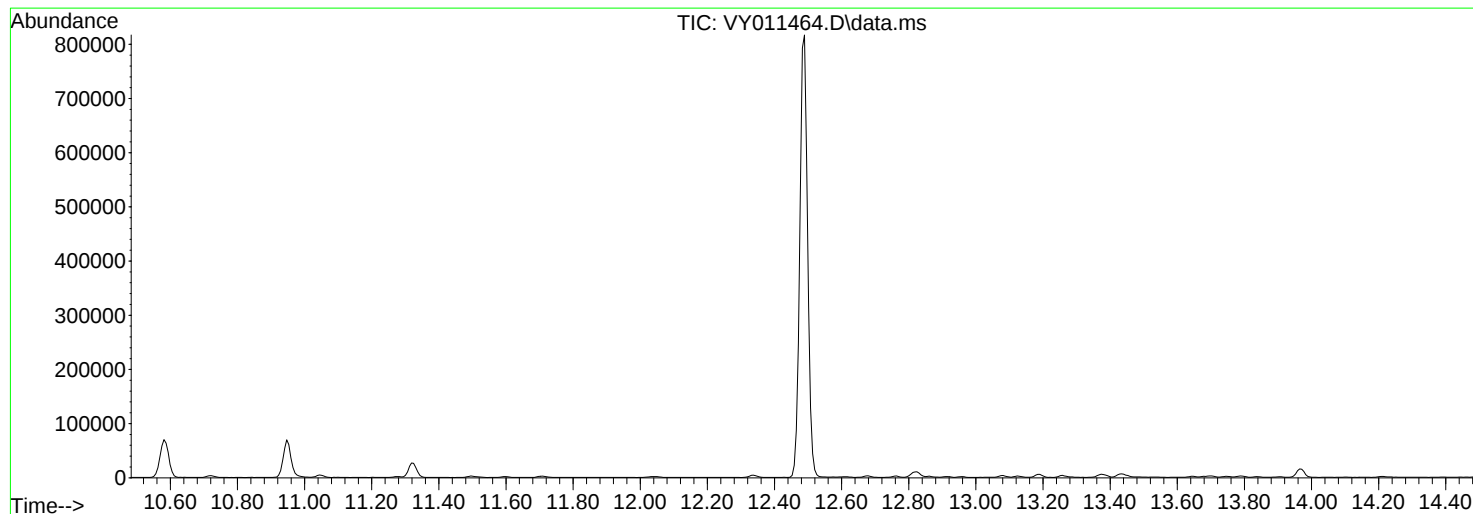

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	21845	PASS
75	95	30	60	47.7	68325	PASS
95	95	100	100	100.0	143323	PASS
96	95	5	9	6.6	9466	PASS
173	174	0.00	2	0.9	1089	PASS
174	95	50	100	82.9	118819	PASS
175	174	5	9	7.3	8692	PASS
176	174	95	101	97.4	115776	PASS
177	176	5	9	7.0	8114	PASS