
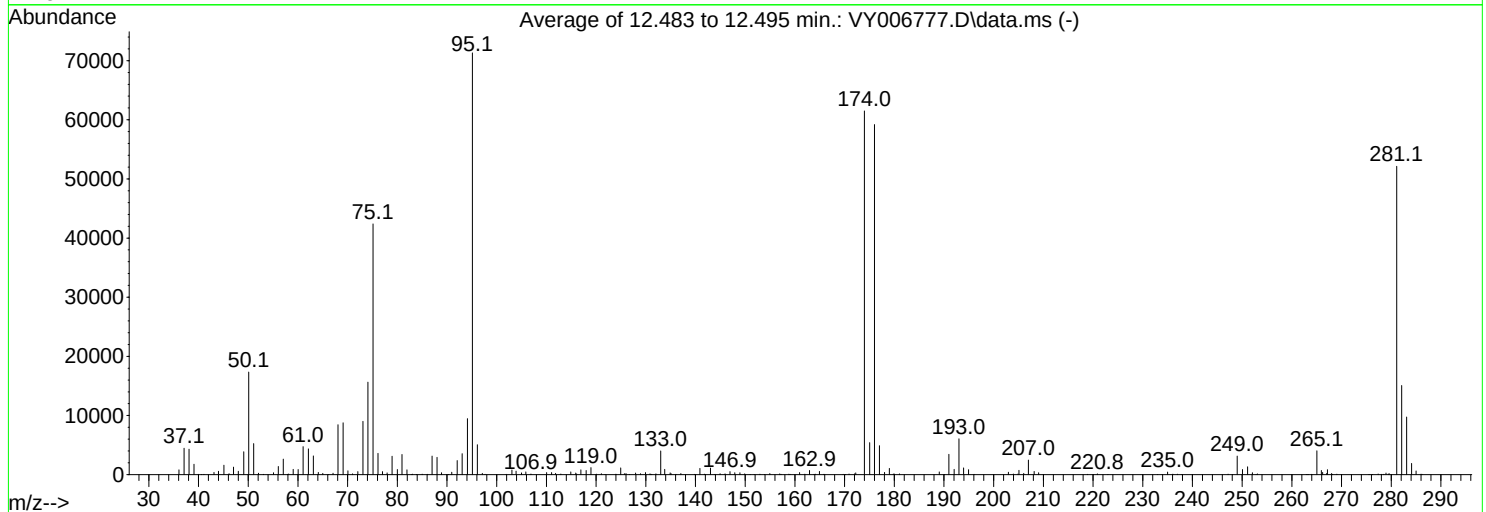


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY111721\
Data File : VY006777.D
Acq On : 17 Nov 2021 09:41
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111521S.M
Title : SW846 8260
Last Update : Tue Nov 16 04:20:03 2021

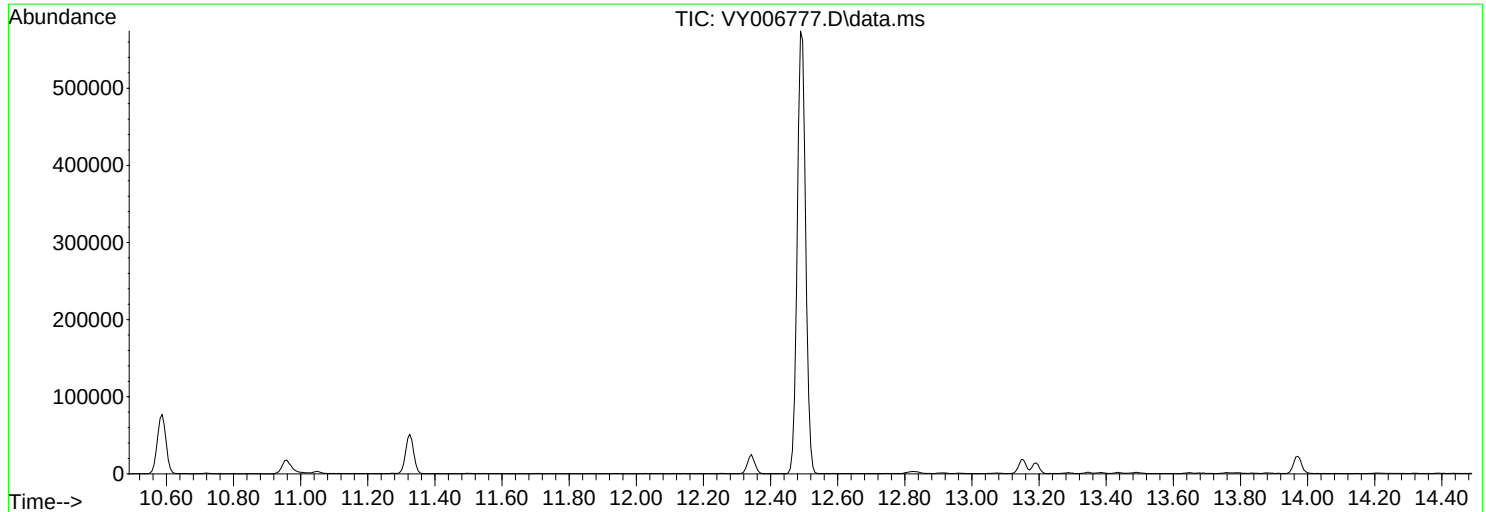

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.3	17353	PASS
75	95	30	60	59.4	42384	PASS
95	95	100	100	100.0	71323	PASS
96	95	5	9	7.1	5055	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.2	61496	PASS
175	174	5	9	8.8	5412	PASS
176	174	95	101	96.3	59195	PASS
177	176	5	9	8.3	4894	PASS