
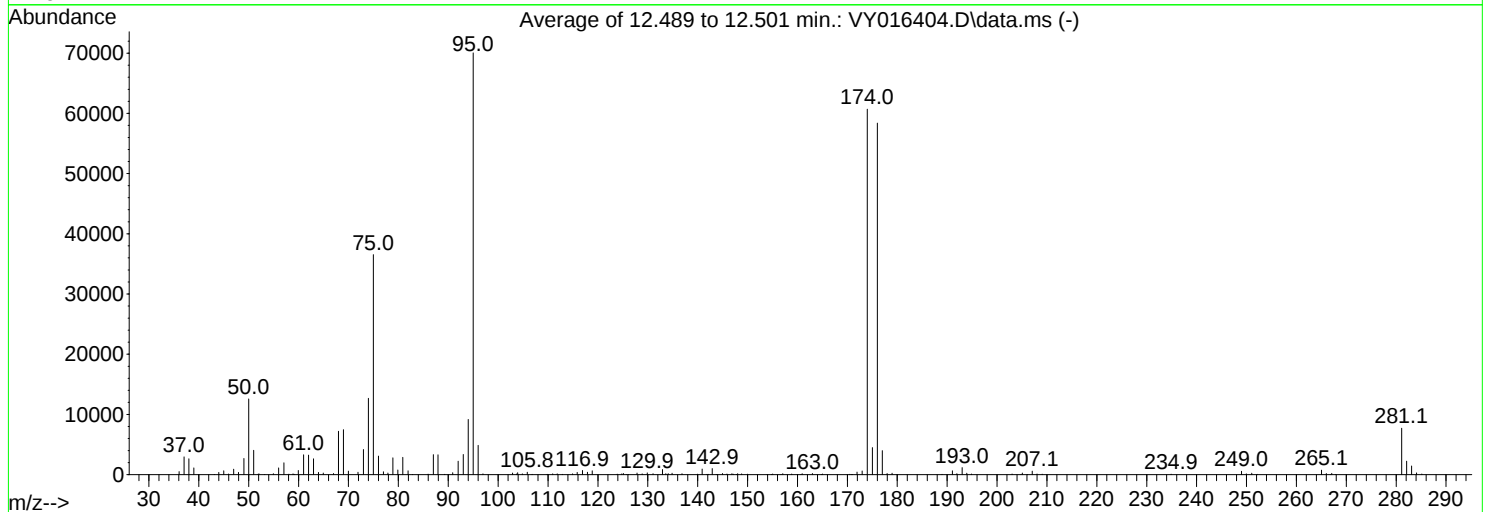


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY111723\
Data File : VY016404.D
Acq On : 17 Nov 2023 07:51
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110823S.M
Title : SW846 8260
Last Update : Thu Nov 09 00:45:52 2023

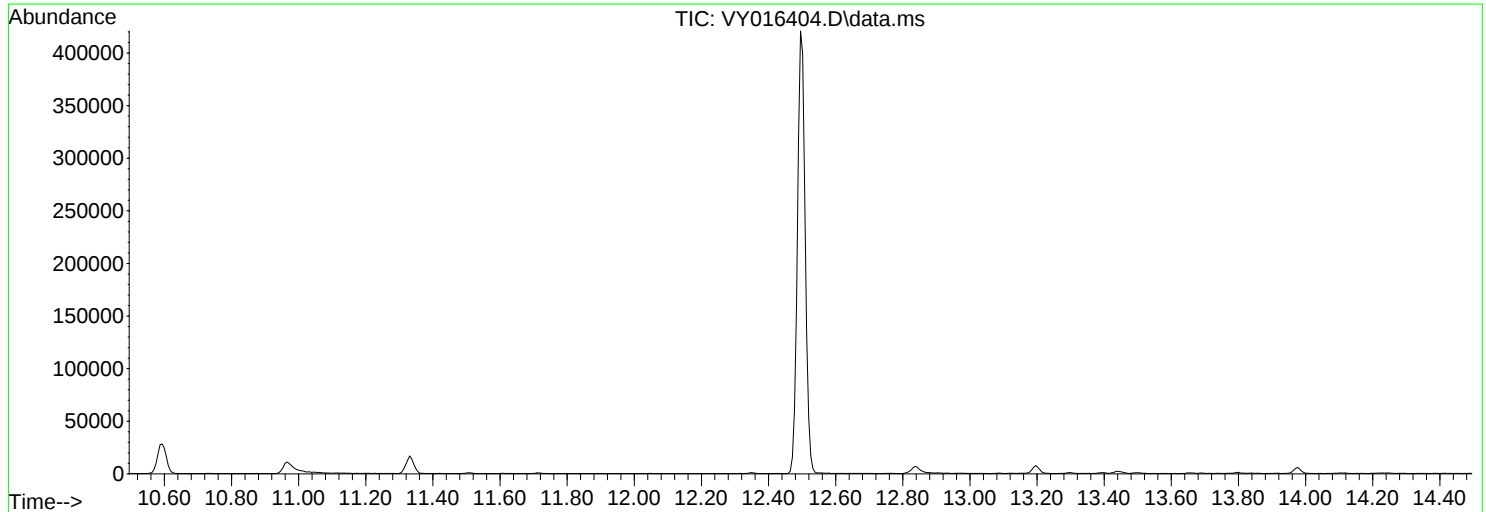

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	12570	PASS
75	95	30	60	52.2	36552	PASS
95	95	100	100	100.0	70053	PASS
96	95	5	9	7.0	4878	PASS
173	174	0.00	2	1.0	613	PASS
174	95	50	100	86.6	60685	PASS
175	174	5	9	7.4	4486	PASS
176	174	95	101	96.2	58381	PASS
177	176	5	9	6.8	3979	PASS