

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY111819\  
 Data File : VY000732.D  
 Acq On : 18 Nov 2019 17:10  
 Operator : SY/MD  
 Sample : K5908-02  
 Misc : 6.52G/5ML/MSVOA Y/SOIL  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 B-8-1-(6-12)

Quant Time: Nov 18 17:56:30 2019  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_Y\METHODS\82Y103019S.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Oct 30 13:30:53 2019  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) Pentafluorobenzene      | 7.80  | 168  | 171600   | 50.00 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.70  | 114  | 321002   | 50.00 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.49 | 117  | 289631   | 50.00 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.42 | 152  | 120728   | 50.00 | ug/l  | 0.00     |

| System Monitoring Compounds | R.T.  | QIon | Response | Conc  | Units   | Dev(Min) |
|-----------------------------|-------|------|----------|-------|---------|----------|
| 33) 1,2-Dichloroethane-d4   | 8.15  | 65   | 110943   | 62.47 | ug/l    | 0.00     |
| Spiked Amount               |       |      |          |       |         |          |
|                             |       |      | Recovery | =     | 124.94% |          |
| 35) Dibromofluoromethane    | 7.73  | 113  | 98295    | 52.16 | ug/l    | 0.00     |
| Spiked Amount               |       |      |          |       |         |          |
|                             |       |      | Recovery | =     | 104.32% |          |
| 50) Toluene-d8              | 10.18 | 98   | 375130   | 52.46 | ug/l    | 0.00     |
| Spiked Amount               |       |      |          |       |         |          |
|                             |       |      | Recovery | =     | 104.92% |          |
| 62) 4-Bromofluorobenzene    | 12.48 | 95   | 123984   | 45.55 | ug/l    | 0.00     |
| Spiked Amount               |       |      |          |       |         |          |
|                             |       |      | Recovery | =     | 91.10%  |          |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY111819\  
Data File : VY000732.D  
Acq On : 18 Nov 2019 17:10  
Operator : SY/MD  
Sample : K5908-02  
Misc : 6.52G/5ML/MSVOA Y/SOIL  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
B-8-1-(6-12)

Quant Time: Nov 18 17:56:30 2019  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_Y\METHODS\82Y103019S.M  
Quant Title : SW846 8260  
QLast Update : Wed Oct 30 13:30:53 2019  
Response via : Initial Calibration

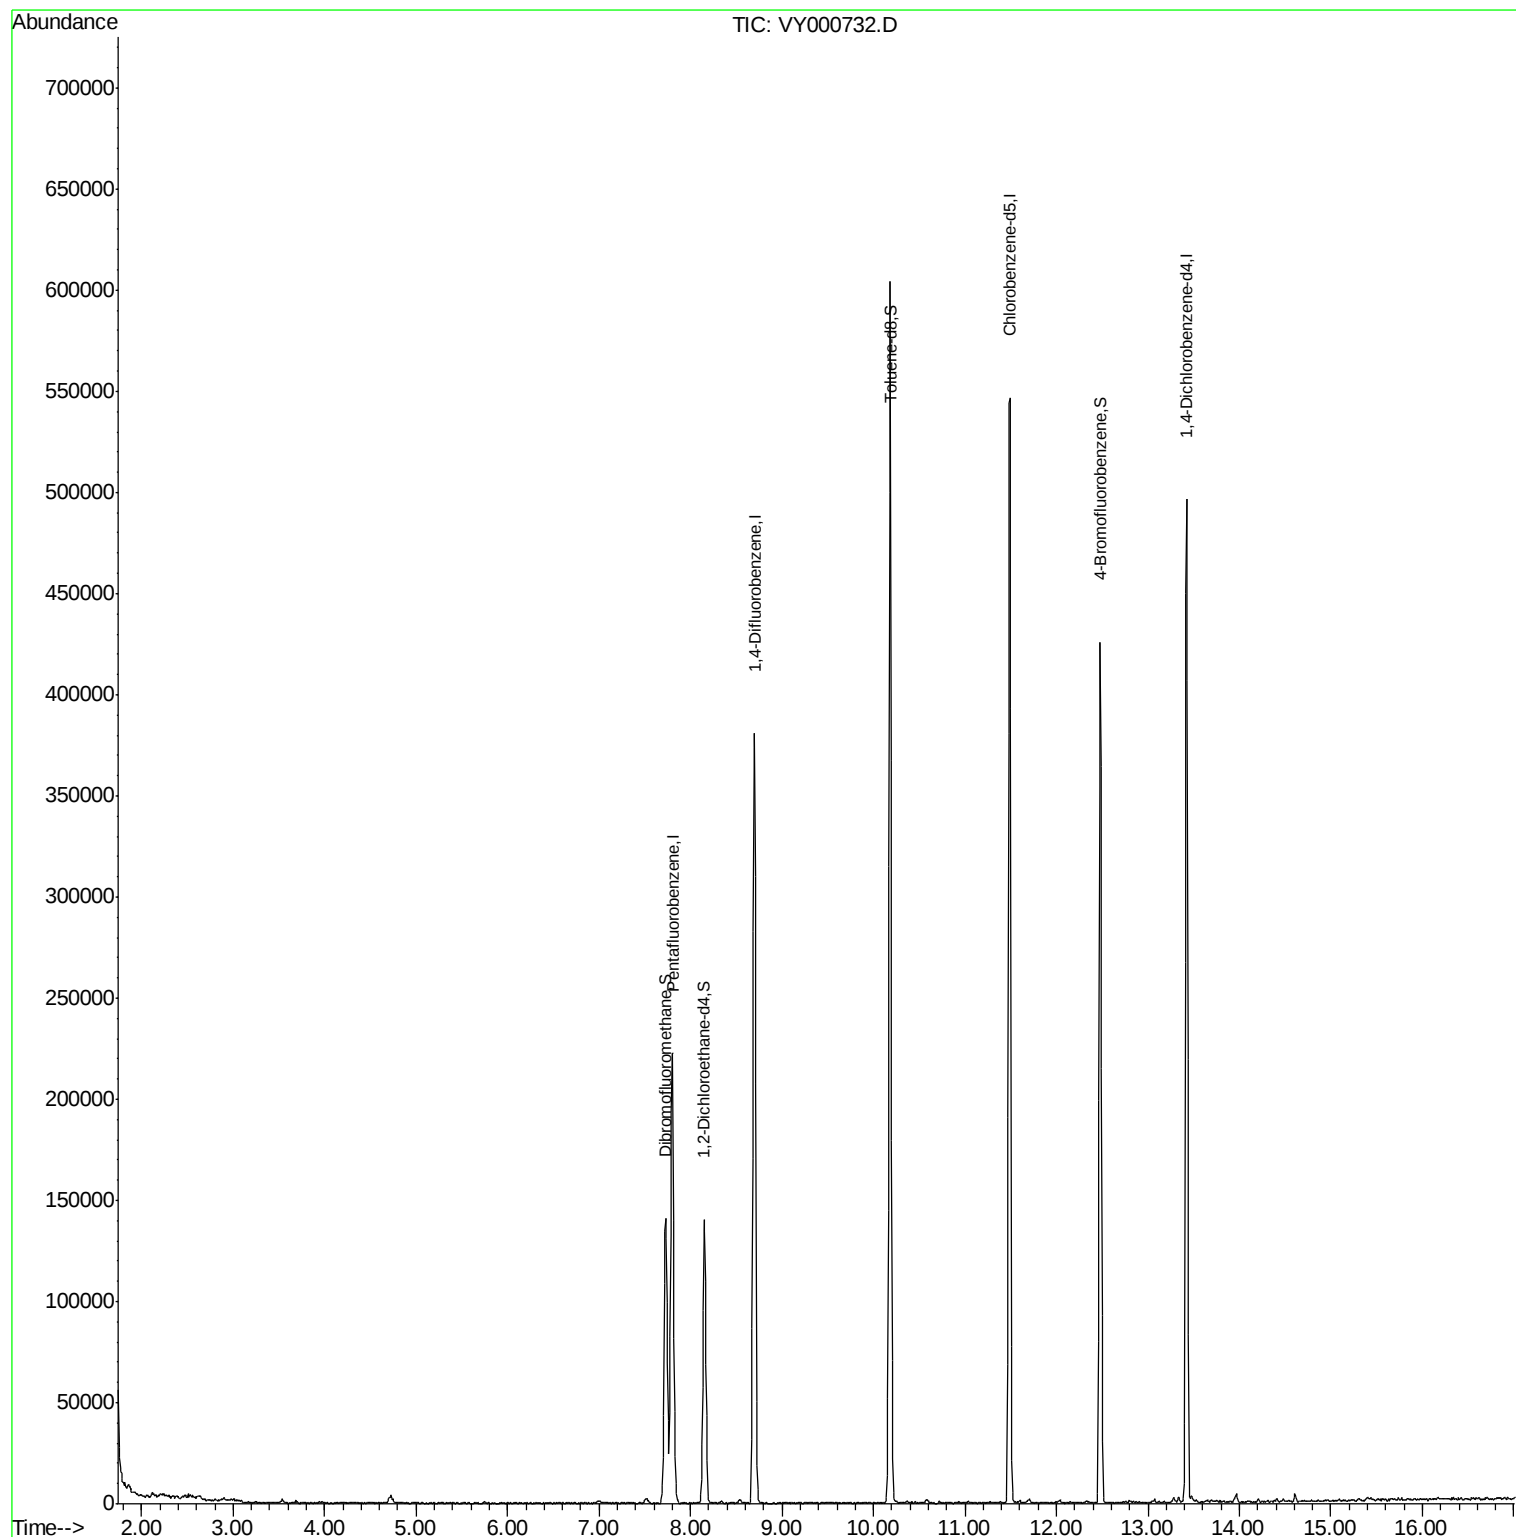



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 995

Delta R.T. 0.00 min

Lab File: VY000732.D

Acq: 18 Nov 2019 17:10

Instrument :

MSVOA\_Y

ClientSampleId :


B-8-1-(6-12)

Tot Ion:168 Resp: 171600

Ion Ratio Lower Upper

168 100

99 57.6 45.7 68.5

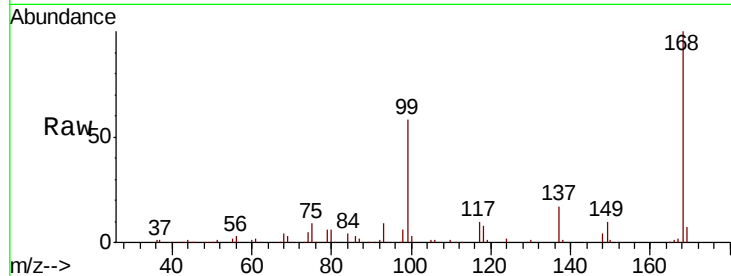

Abundance Ion 167.90 (167.60 to 168.60): VY000732.D (-946) (-)

Ion 98.90 (98.60 to 99.60): VY000732.D (-946) (-)

7.80

80000



60000

40000

20000

0

Time-->

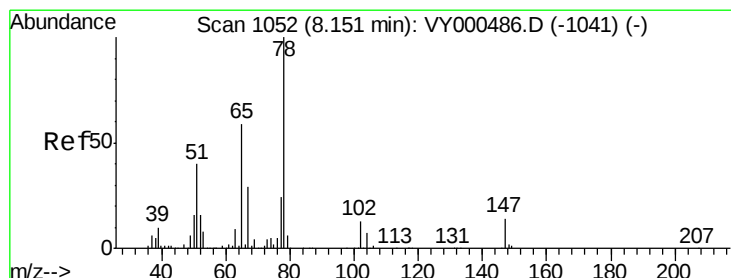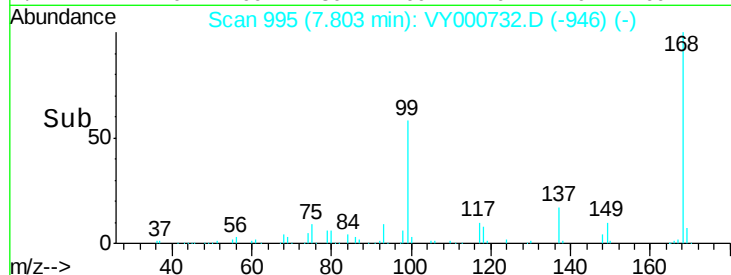

#33

1,2-Dichloroethane-d4

Concen: 62.474 ug/l

RT: 8.15 min Scan# 1052

Delta R.T. 0.00 min

Lab File: VY000732.D


Acq: 18 Nov 2019 17:10

Tgt Ion: 65 Resp: 110943

Ion Ratio Lower Upper

65 100

67 51.7 0.0 107.2

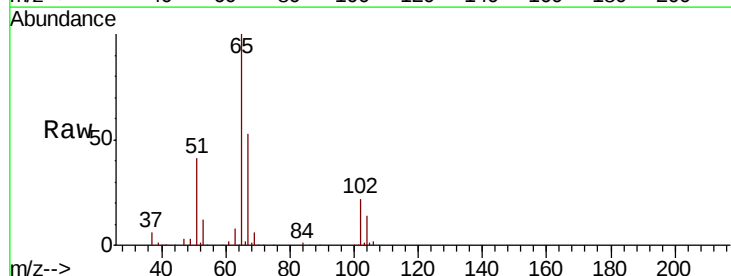

Abundance Ion 64.90 (64.60 to 65.60): VY000732.D (-1003) (-)

Ion 66.90 (66.60 to 67.60): VY000732.D (-1003) (-)

8.15

50000

40000


30000


20000

10000

0

Time-->

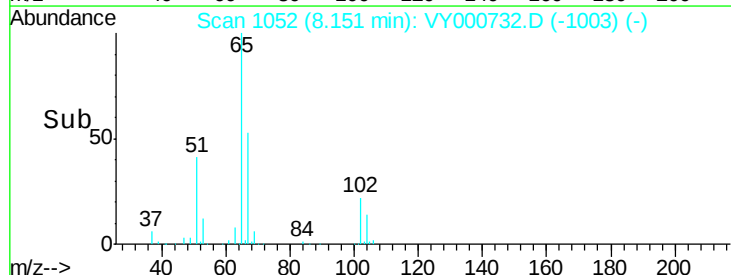

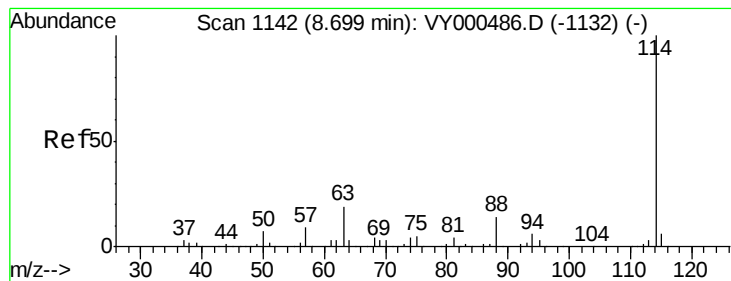

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.70 min Scan# 1142

Delta R.T. 0.00 min

Lab File: VY000732.D

Acq: 18 Nov 2019 17:10

Instrument :

MSVOA\_Y

ClientSampleId :

B-8-1-(6-12)


Tot Ion:114 Resp: 321002

Ion Ratio Lower Upper

114 100

63 20.7 0.0 38.0




88 15.6 0.0 28.6

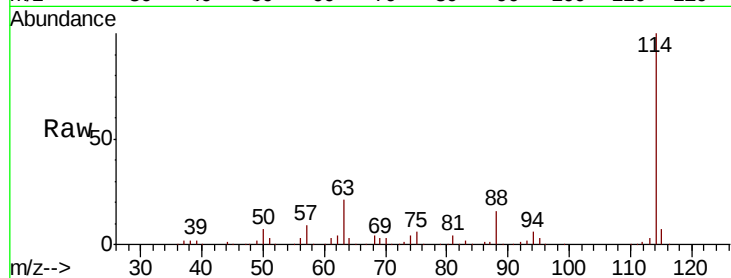

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VY0

Ion 87.90 (87.60 to 88.60): VY0

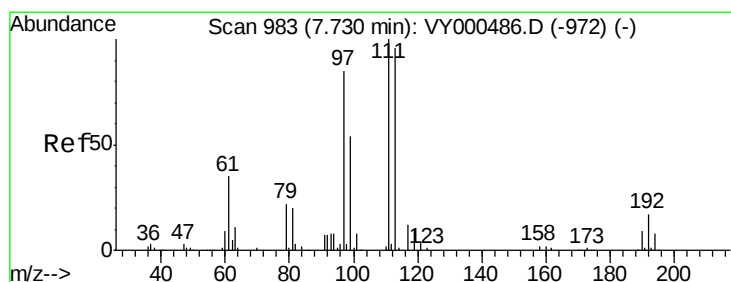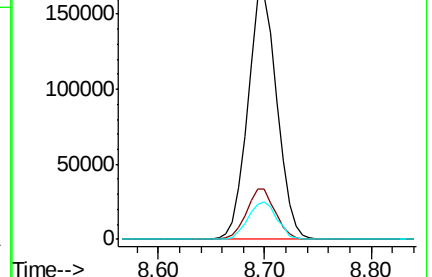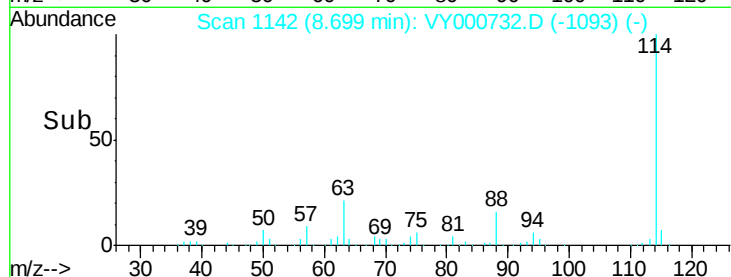

#35

Dibromofluoromethane

Concen: 52.160 ug/l

RT: 7.73 min Scan# 983

Delta R.T. 0.00 min

Lab File: VY000732.D

Acq: 18 Nov 2019 17:10


Tgt Ion:113 Resp: 98295

Ion Ratio Lower Upper

113 100

111 103.3 81.7 122.5



192 19.9 15.0 22.4

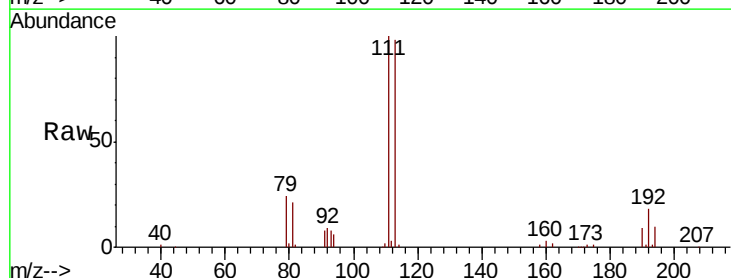


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

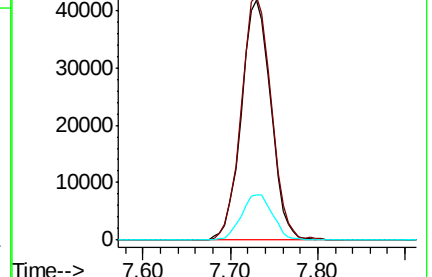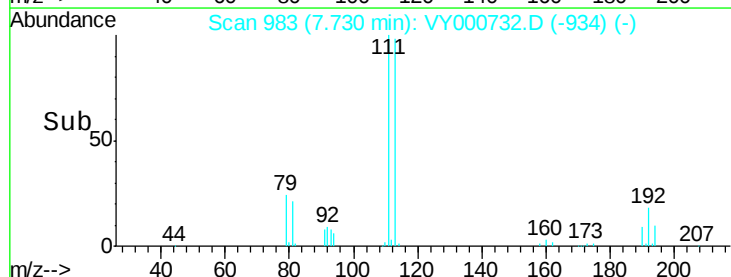

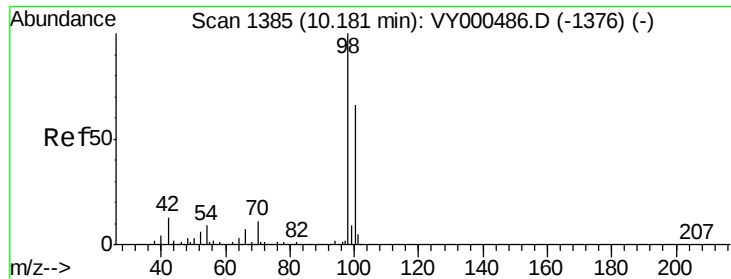

#50

Toluene-d8

Concen: 52.461 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. 0.00 min

Lab File: VY000732.D

Acq: 18 Nov 2019 17:10

Instrument :

MSVOA\_Y

ClientSampleId :





B-8-1-(6-12)

Tot Ion: 98 Resp: 375130

Ion Ratio Lower Upper

98 100

100 67.8 52.9 79.3

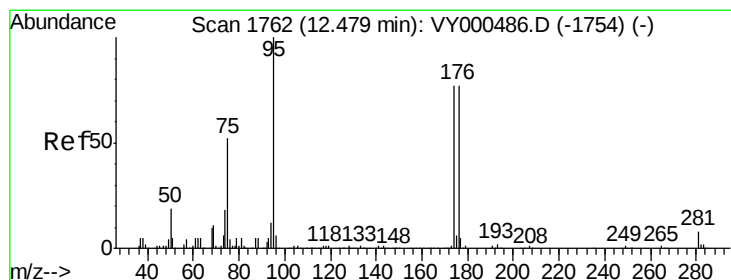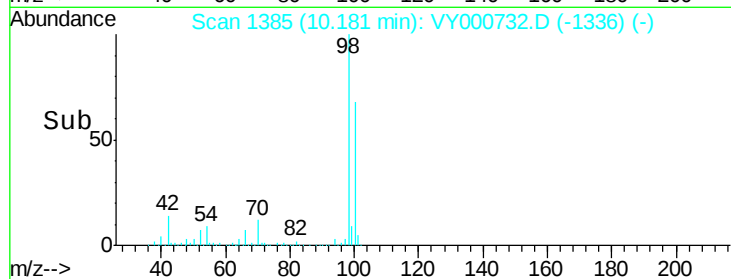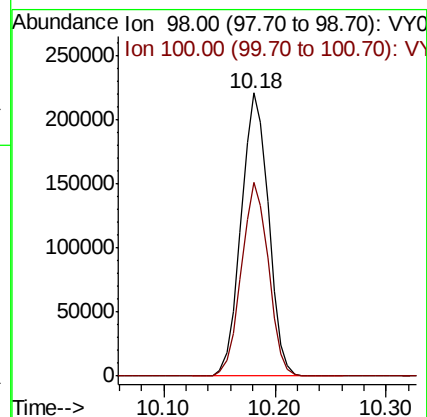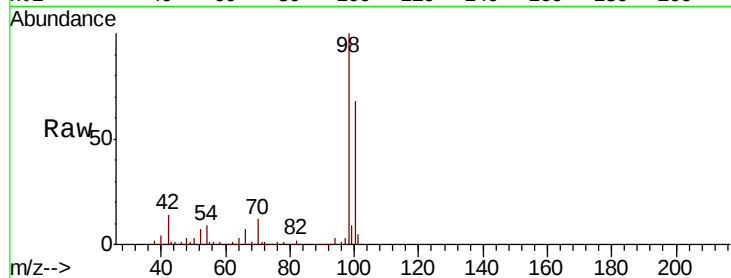

#62

4-Bromofluorobenzene

Concen: 45.545 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. 0.00 min

Lab File: VY000732.D

Acq: 18 Nov 2019 17:10




Tgt Ion: 95 Resp: 123984

Ion Ratio Lower Upper

95 100

174 81.9 0.0 161.6

176 79.3 0.0 157.8

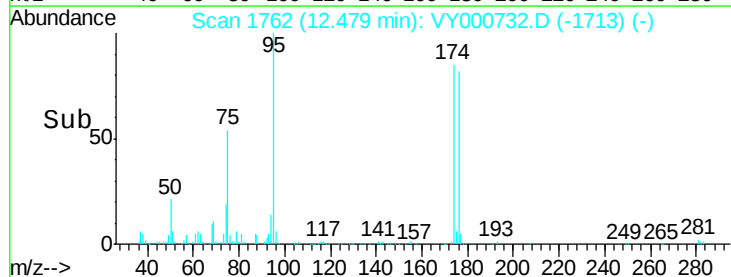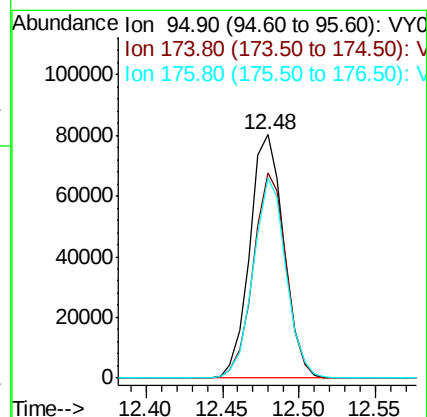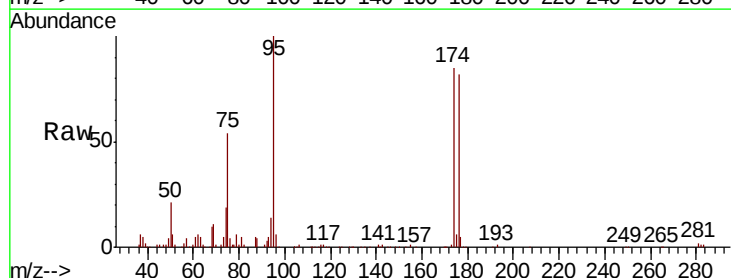







#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.49 min Scan# 1600  
Delta R.T. 0.00 min  
Lab File: VY000732.D  
Acq: 18 Nov 2019 17:10

Instrument :  
MSVOA\_Y  
ClientSampleId :  
B-8-1-(6-12)

Tot Ion:117 Resp: 289631  
Ion Ratio Lower Upper  
117 100  
82 53.9 40.8 61.2  
119 31.8 26.2 39.2

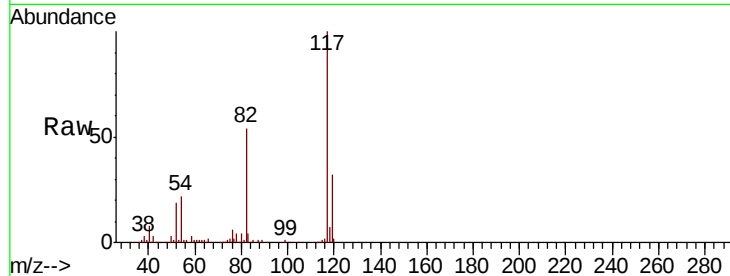


Abundance Ion 116.90 (116.60 to 117.60): V  
Ion 82.00 (81.70 to 82.70): VY0  
Ion 118.90 (118.60 to 119.60): V

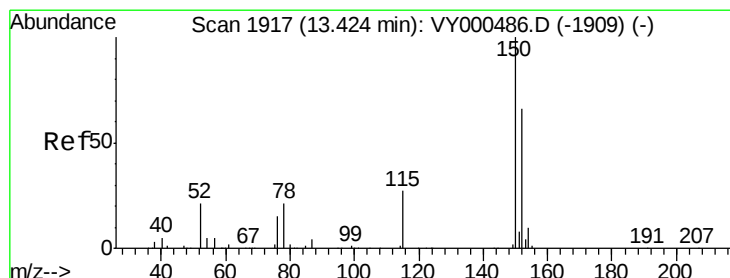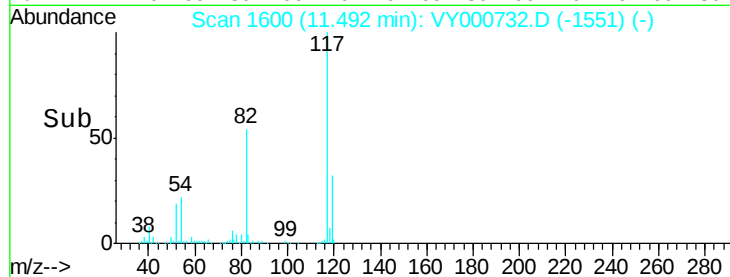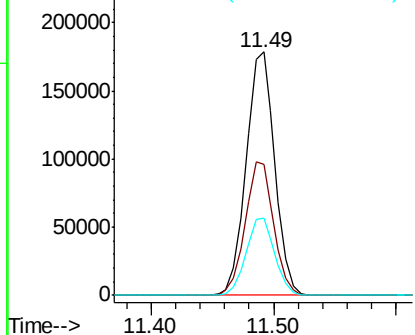

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.42 min Scan# 1917  
Delta R.T. 0.00 min  
Lab File: VY000732.D  
Acq: 18 Nov 2019 17:10

Tgt Ion:152 Resp: 120728  
Ion Ratio Lower Upper  
152 100  
115 58.2 29.1 87.4  
150 157.1 0.0 348.8

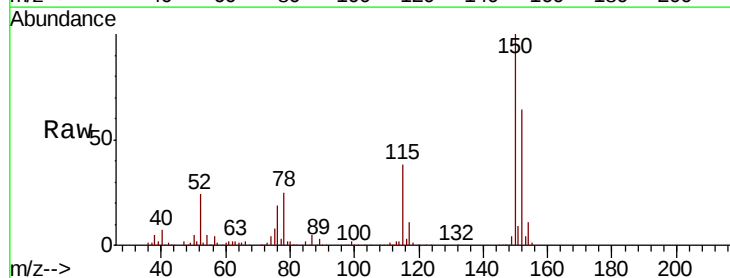

Abundance Ion 151.90 (151.60 to 152.60): V  
Ion 114.90 (114.60 to 115.60): V  
Ion 149.90 (149.60 to 150.60): V

