


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv111919\
Data File : VY000736.D
Acq On : 19 Nov 2019 09:40
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
Title : SW846 8260
Last Update : Wed Oct 30 13:30:53 2019

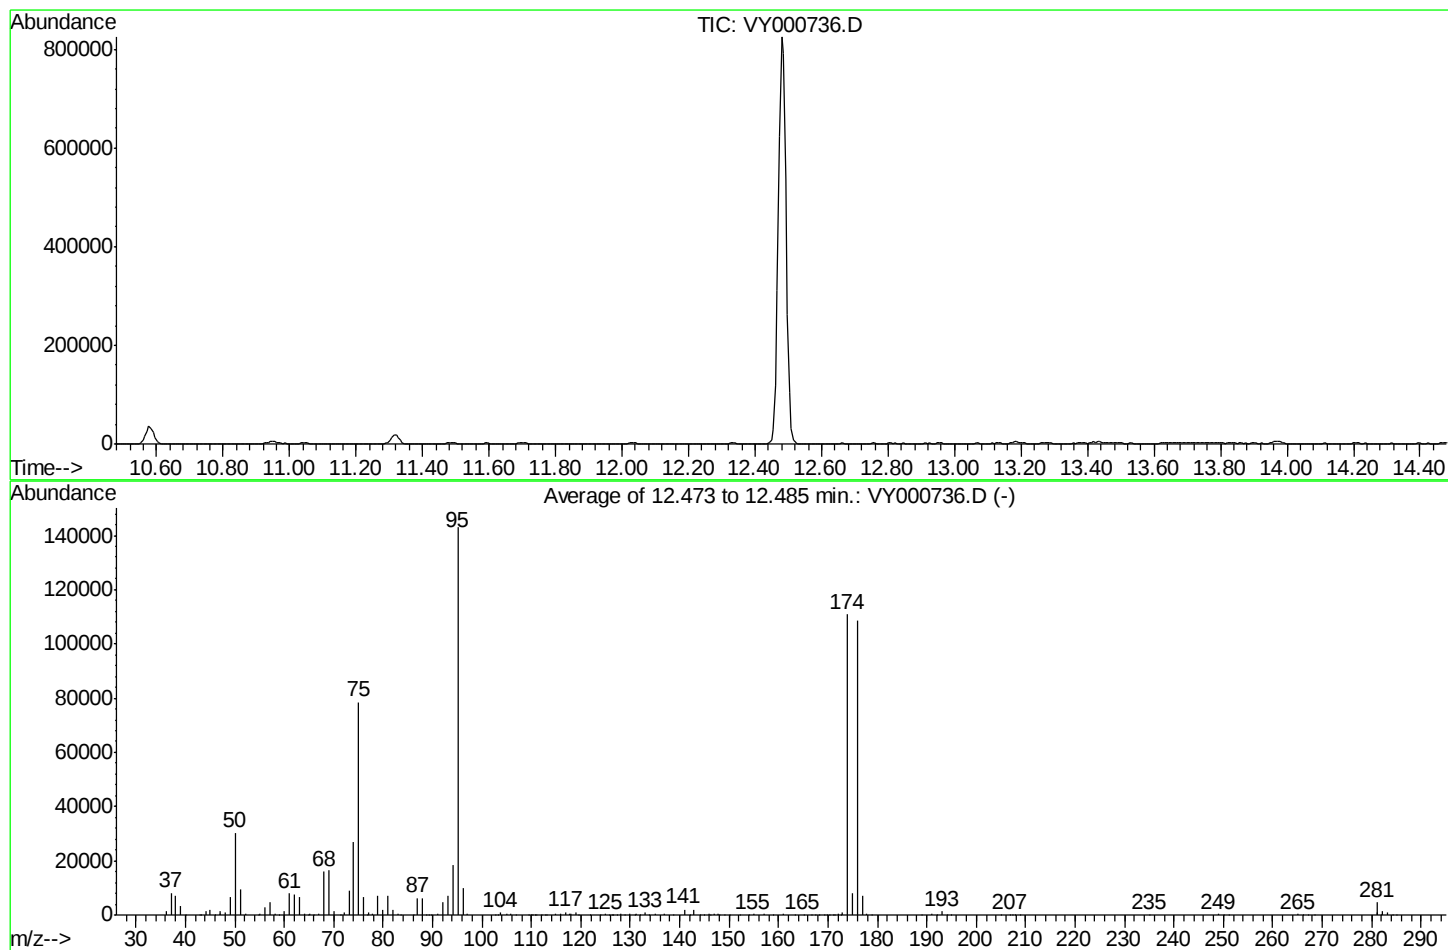

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	30234	PASS
75	95	30	60	54.8	78397	PASS
95	95	100	100	100.0	143010	PASS
96	95	5	9	6.9	9850	PASS
173	174	0.00	2	0.7	808	PASS
174	95	50	100	77.5	110842	PASS
175	174	5	9	7.2	7953	PASS
176	174	95	101	97.9	108469	PASS
177	176	5	9	6.6	7189	PASS