


Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY112020\
 Data File : VY003556.D
 Acq On : 20 Nov 2020 09:12
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/10ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y112020S.M
 Title : SW846 8260
 Last Update : Sat Nov 21 01:00:42 2020

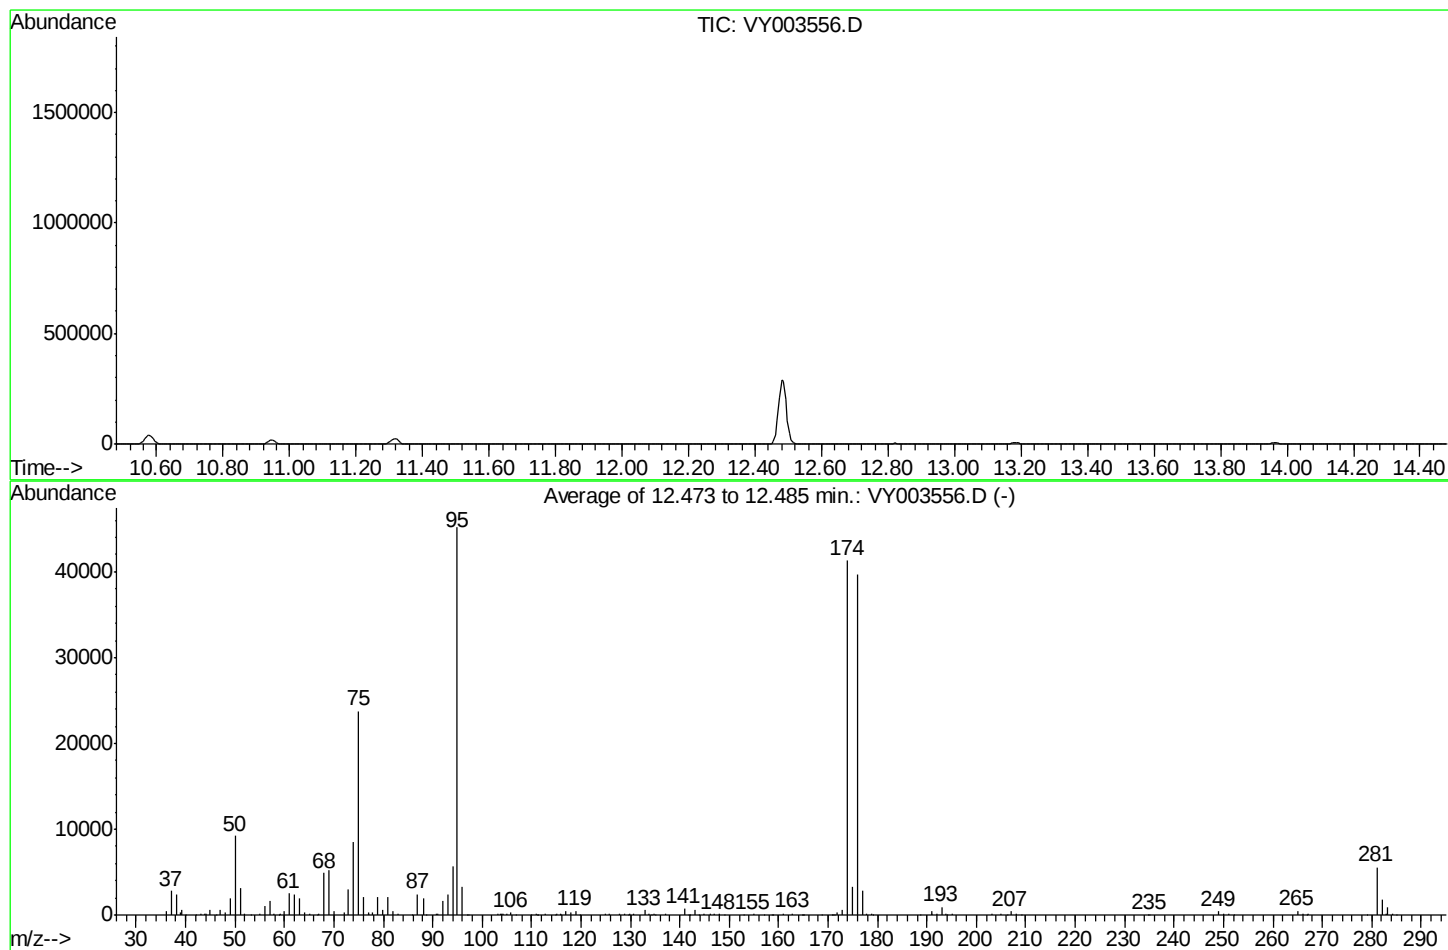

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	9234	PASS
75	95	30	60	52.6	23752	PASS
95	95	100	100	100.0	45178	PASS
96	95	5	9	7.2	3238	PASS
173	174	0.00	2	1.4	592	PASS
174	95	50	100	91.3	41261	PASS
175	174	5	9	7.9	3247	PASS
176	174	95	101	96.1	39645	PASS
177	176	5	9	7.0	2782	PASS