
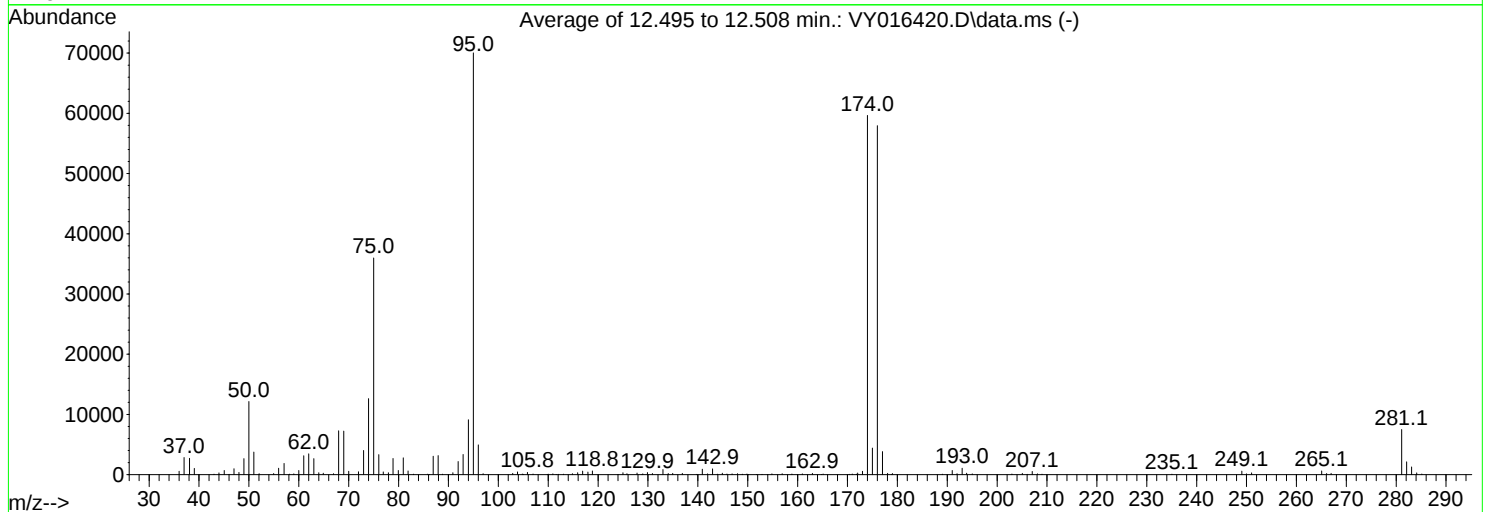


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112023\
Data File : VY016420.D
Acq On : 20 Nov 2023 08:59
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110823S.M
Title : SW846 8260
Last Update : Thu Nov 09 00:45:52 2023

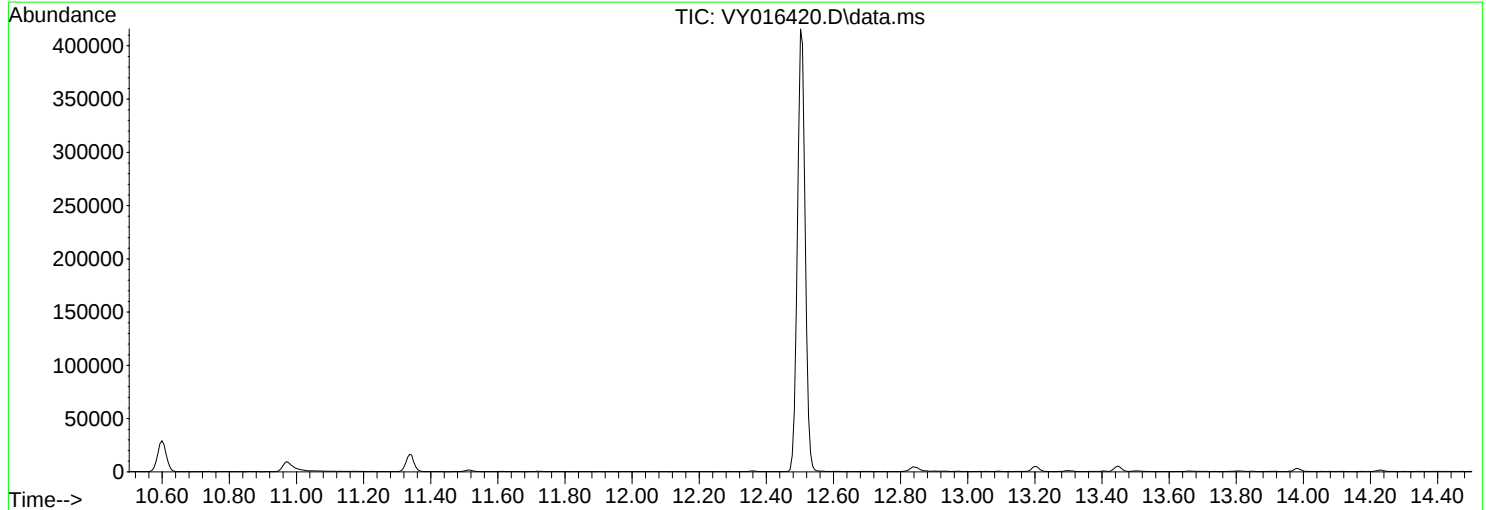

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	12158	PASS
75	95	30	60	51.4	35987	PASS
95	95	100	100	100.0	70043	PASS
96	95	5	9	7.1	4948	PASS
173	174	0.00	2	1.0	575	PASS
174	95	50	100	85.2	59645	PASS
175	174	5	9	7.4	4421	PASS
176	174	95	101	97.1	57939	PASS
177	176	5	9	6.6	3831	PASS