


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv112119\
Data File : VY000761.D
Acq On : 21 Nov 2019 11:30
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
Title : SW846 8260
Last Update : Wed Oct 30 13:30:53 2019

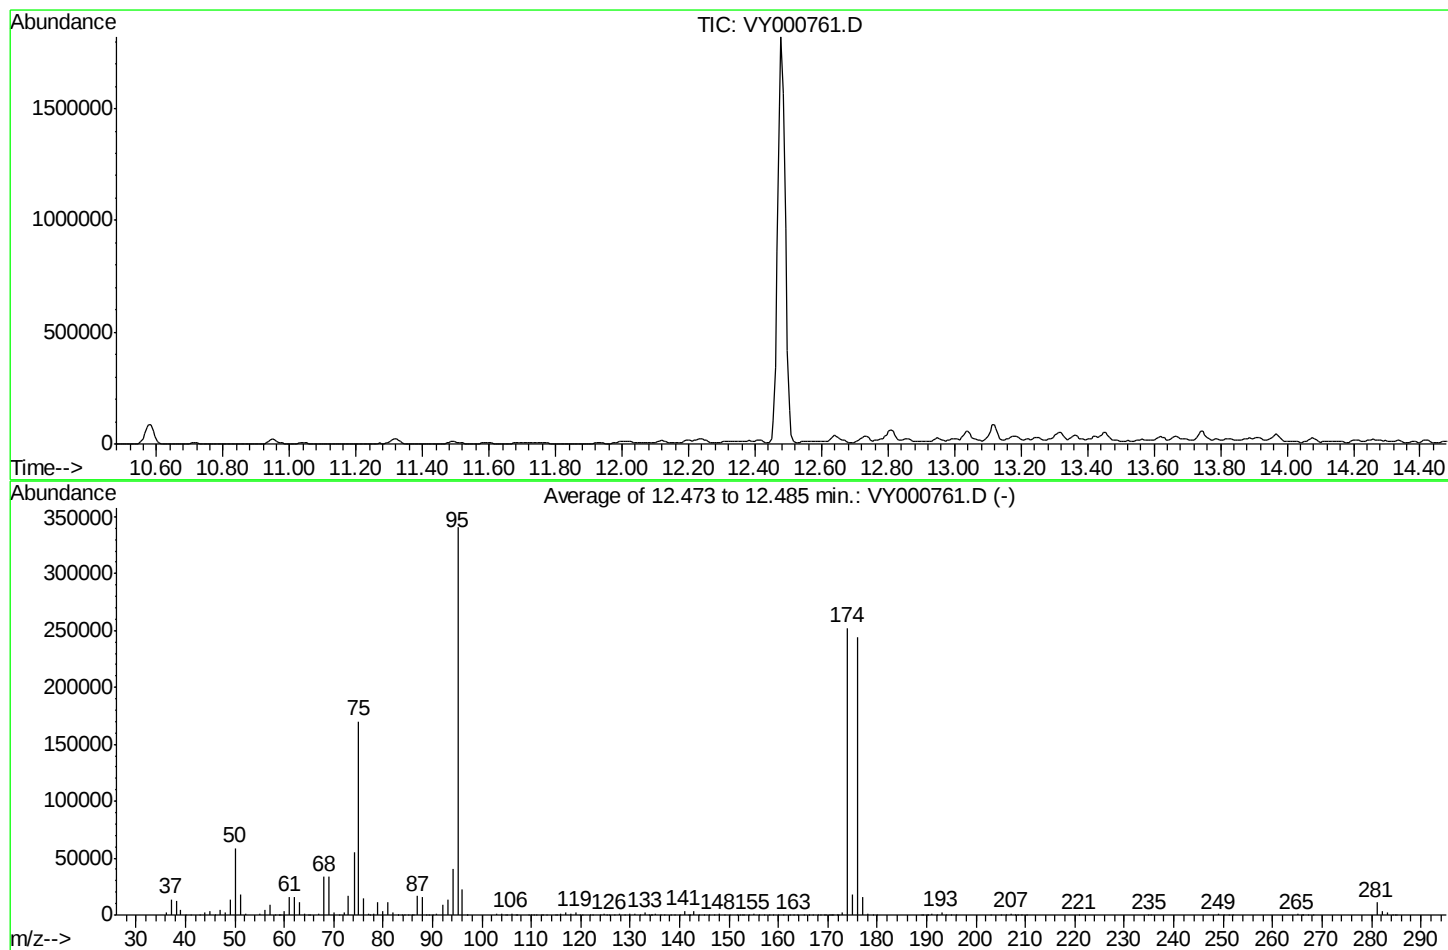

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1754

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	58536	PASS
75	95	30	60	50.0	170453	PASS
95	95	100	100	100.0	340693	PASS
96	95	5	9	6.8	23092	PASS
173	174	0.00	2	0.7	1868	PASS
174	95	50	100	74.0	252138	PASS
175	174	5	9	7.2	18065	PASS
176	174	95	101	96.9	244394	PASS
177	176	5	9	6.6	16227	PASS