
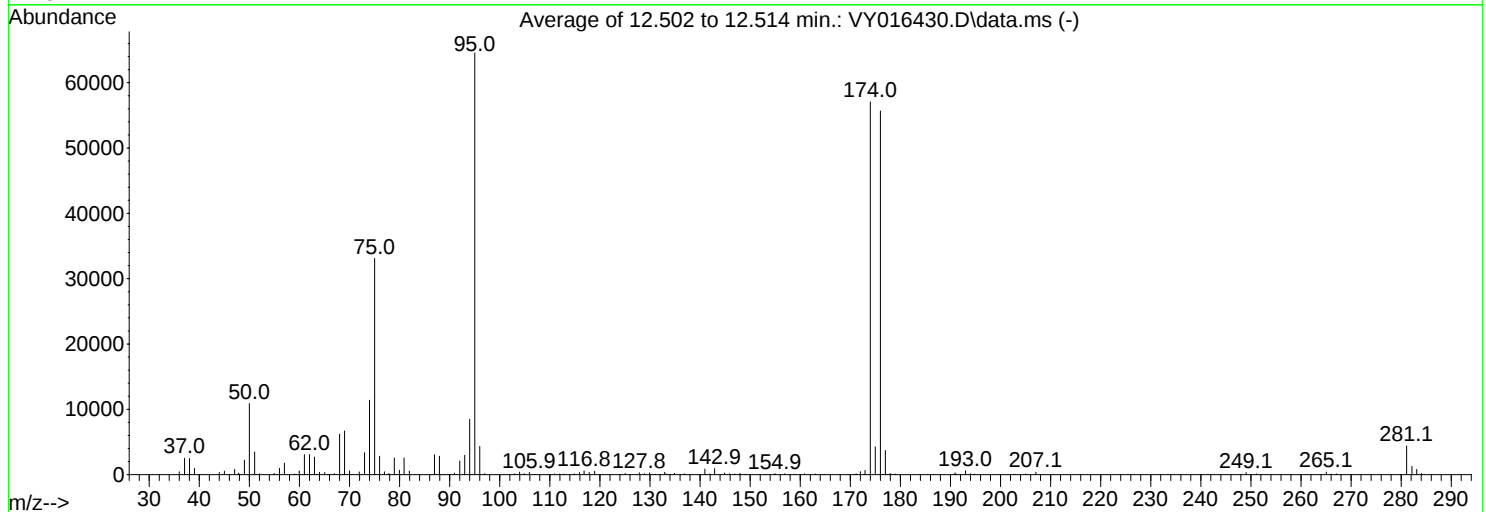


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112123\
Data File : VY016430.D
Acq On : 21 Nov 2023 07:44
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110823S.M
Title : SW846 8260
Last Update : Thu Nov 09 00:45:52 2023

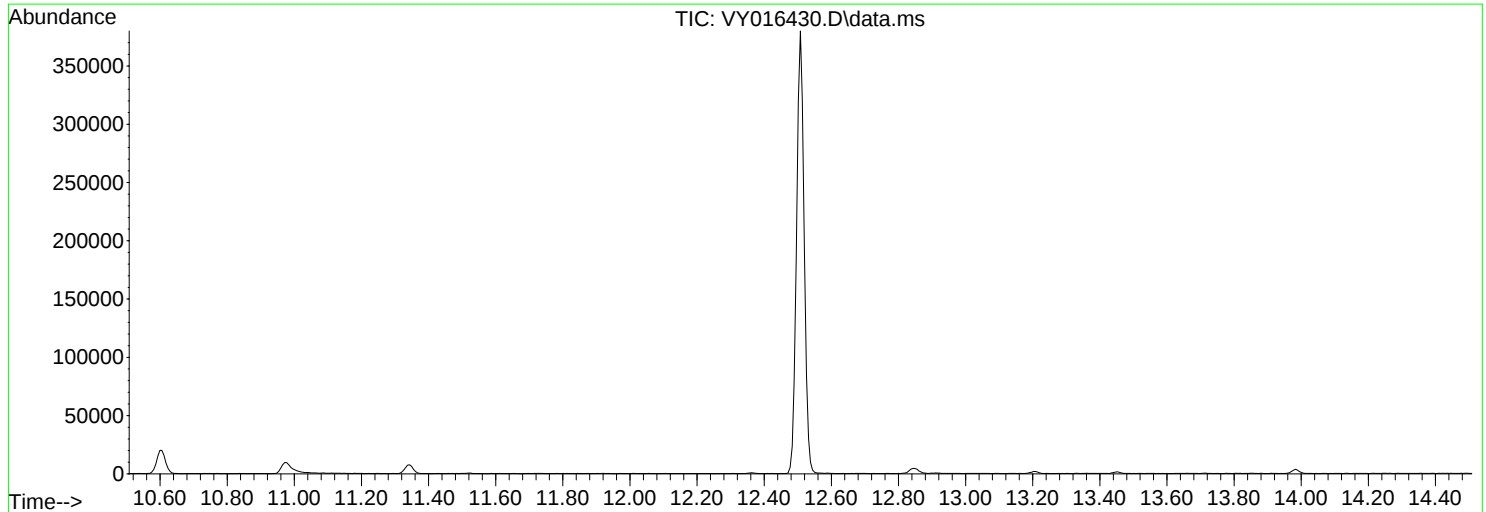

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	10888	PASS
75	95	30	60	51.3	33099	PASS
95	95	100	100	100.0	64573	PASS
96	95	5	9	6.7	4314	PASS
173	174	0.00	2	1.2	665	PASS
174	95	50	100	88.4	57085	PASS
175	174	5	9	7.5	4271	PASS
176	174	95	101	97.5	55683	PASS
177	176	5	9	6.6	3689	PASS