


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv112219\
Data File : VY000780.D
Acq On : 22 Nov 2019 09:38
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
Title : SW846 8260
Last Update : Wed Oct 30 13:30:53 2019

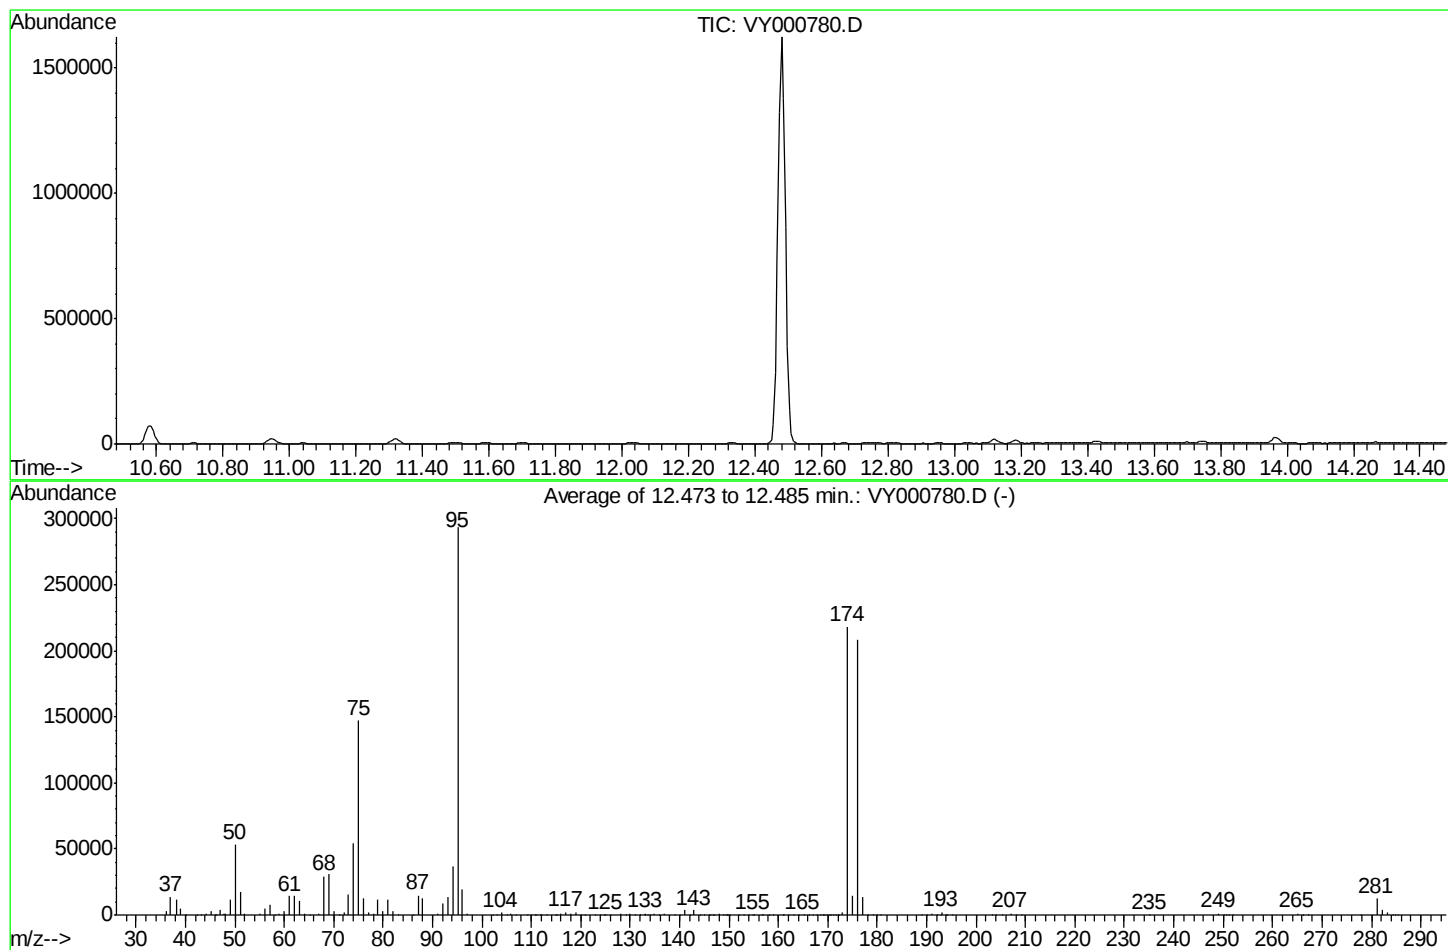

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	53208	PASS
75	95	30	60	50.1	146944	PASS
95	95	100	100	100.0	293376	PASS
96	95	5	9	6.5	19074	PASS
173	174	0.00	2	0.8	1717	PASS
174	95	50	100	74.3	218026	PASS
175	174	5	9	6.8	14815	PASS
176	174	95	101	95.7	208704	PASS
177	176	5	9	6.7	13916	PASS