

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112222\
 Data File : VY011541.D
 Acq On : 22 Nov 2022 12:30
 Operator : KP/MD
 Sample : N5698-03
 Misc : 5.04g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BANK-RUN-SOIL-SAMPLE-3

Quant Time: Nov 23 04:06:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111822S.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 19 22:37:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	143444	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	273387	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	249863	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	101067	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	92167	63.279	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	126.560%
35) Dibromofluoromethane	7.722	113	88282	52.457	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	104.920%
50) Toluene-d8	10.179	98	334324	54.667	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	109.340%
62) 4-Bromofluorobenzene	12.483	95	98520	43.571	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	87.140%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112222\
Data File : VY011541.D
Acq On : 22 Nov 2022 12:30
Operator : KP/MD
Sample : N5698-03
Misc : 5.04g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BANK-RUN-SOIL-SAMPLE-3

Quant Time: Nov 23 04:06:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111822S.M
Quant Title : SW846 8260
QLast Update : Sat Nov 19 22:37:14 2022
Response via : Initial Calibration




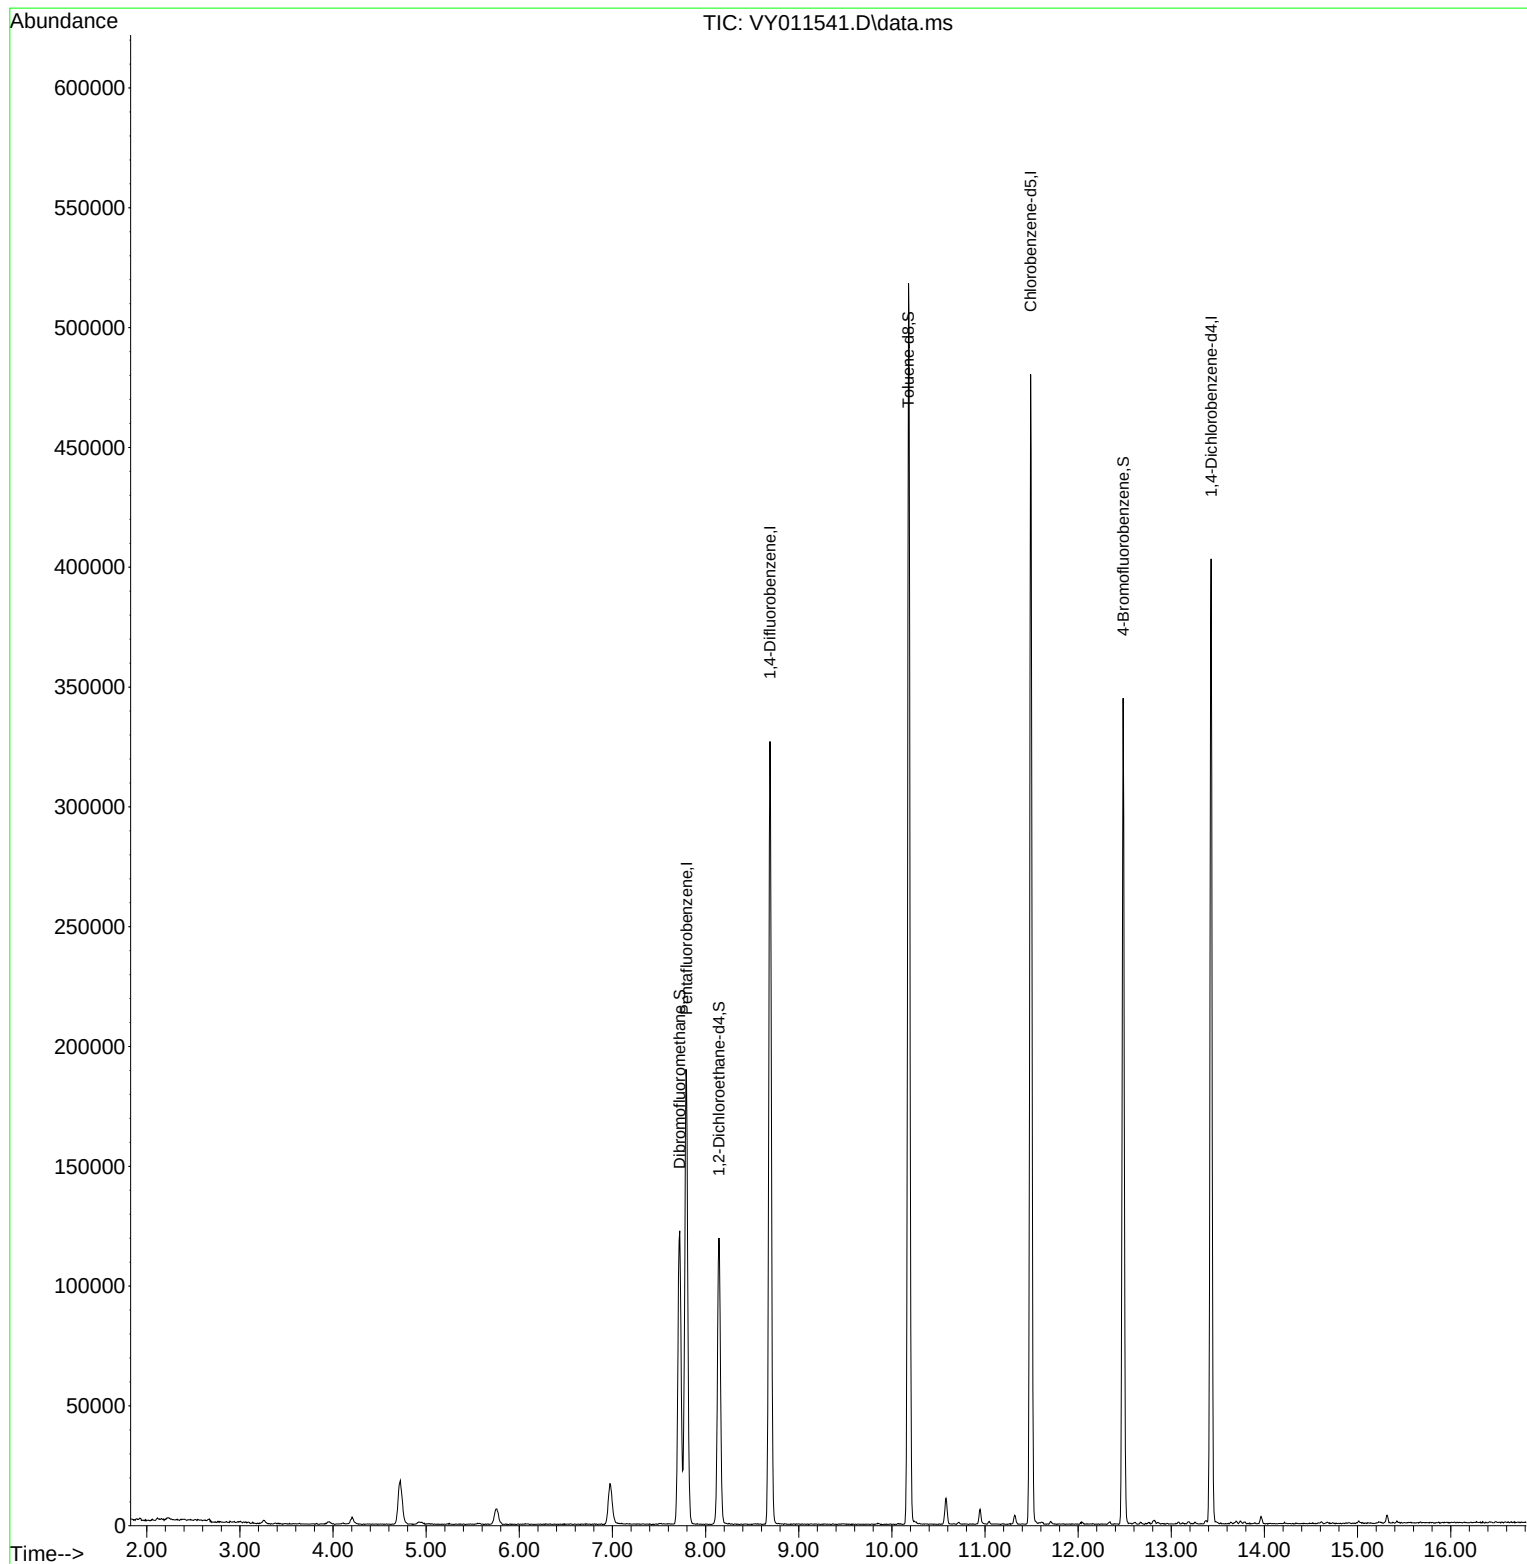


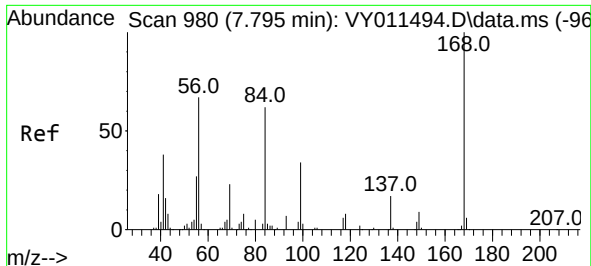

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.000 min
Lab File: VY011541.D
Acq: 22 Nov 2022 12:30




Instrument :
MSVOA_Y
ClientSampleId :
BANK-RUN-SOIL-SAMPLE-3


Tgt Ion:168 Resp: 143444
Ion Ratio Lower Upper
168 100
99 57.8 46.9 70.3

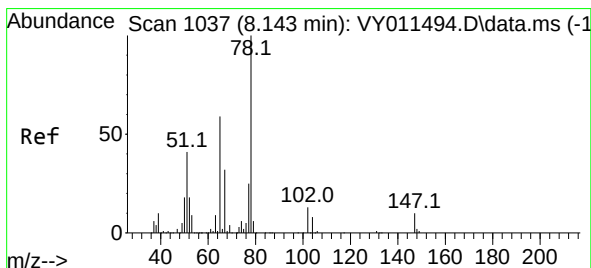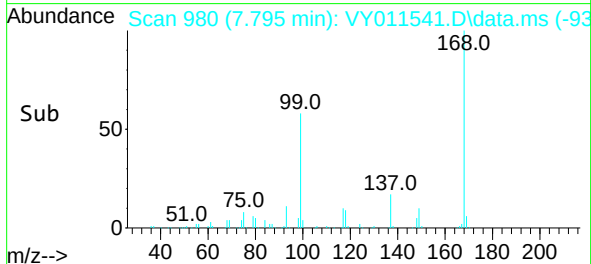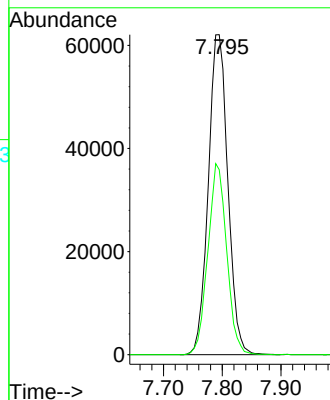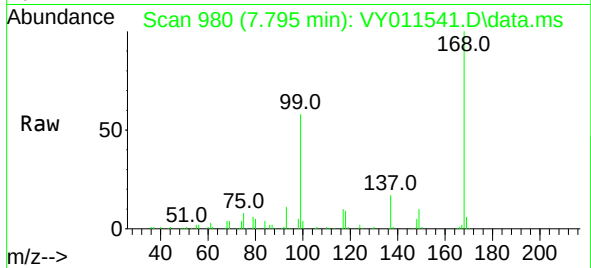

#33
1,2-Dichloroethane-d4
Concen: 63.279 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. -0.001 min
Lab File: VY011541.D
Acq: 22 Nov 2022 12:30

Tgt Ion: 65 Resp: 92167
Ion Ratio Lower Upper
65 100
67 53.7 0.0 99.4


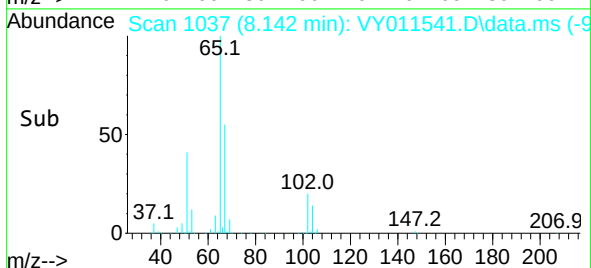
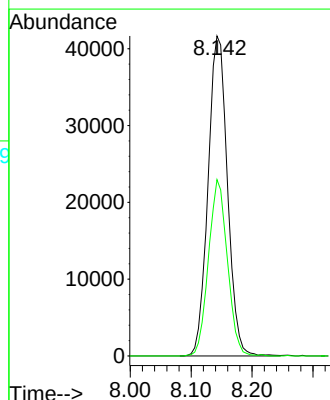
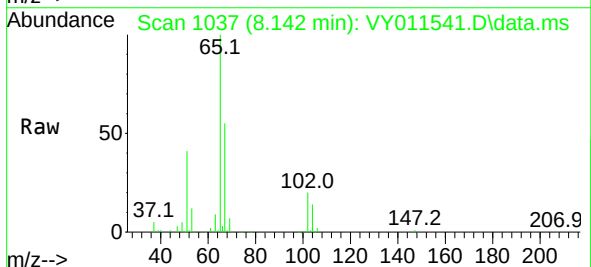


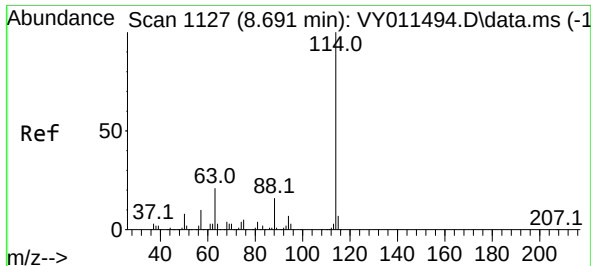

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VY011541.D
Acq: 22 Nov 2022 12:30




Instrument :
MSVOA_Y
ClientSampleId :
BANK-RUN-SOIL-SAMPLE-3


Tgt Ion:114 Resp: 273387
Ion Ratio Lower Upper
114 100
63 21.4 0.0 43.2
88 15.5 0.0 31.8

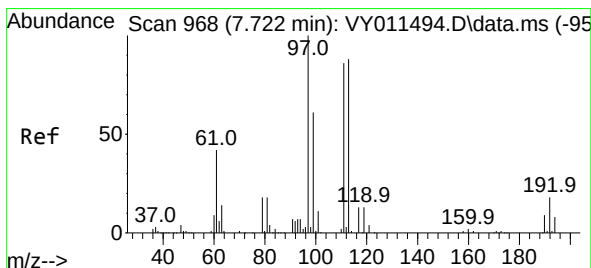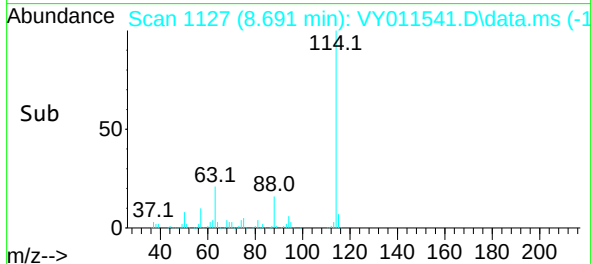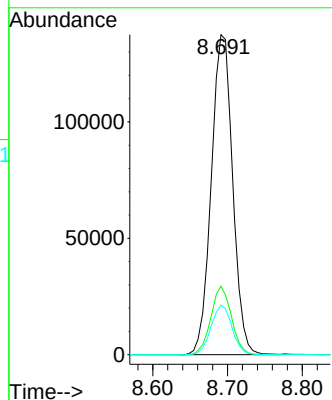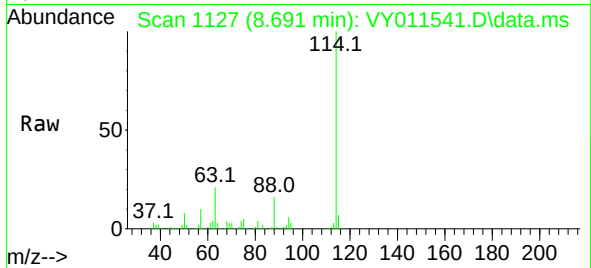

#35
Dibromofluoromethane
Concen: 52.457 ug/l
RT: 7.722 min Scan# 968
Delta R.T. -0.000 min
Lab File: VY011541.D
Acq: 22 Nov 2022 12:30

Tgt Ion:113 Resp: 88282
Ion Ratio Lower Upper
113 100
111 102.7 82.6 124.0
192 19.6 17.6 26.4


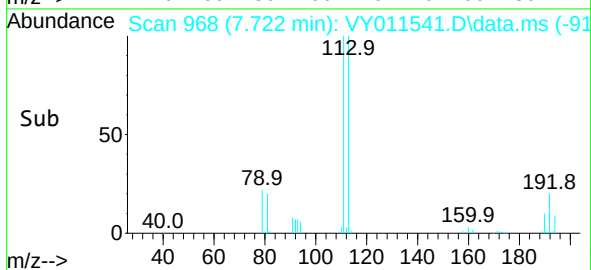
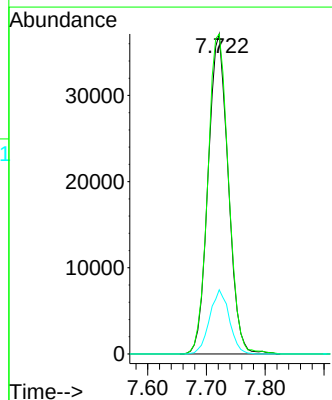
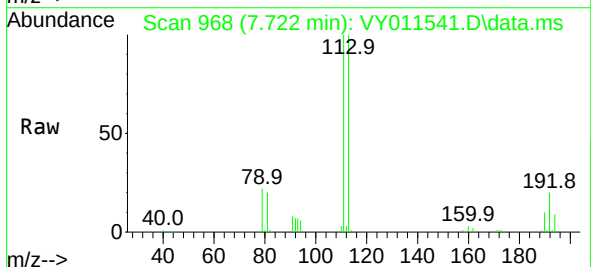


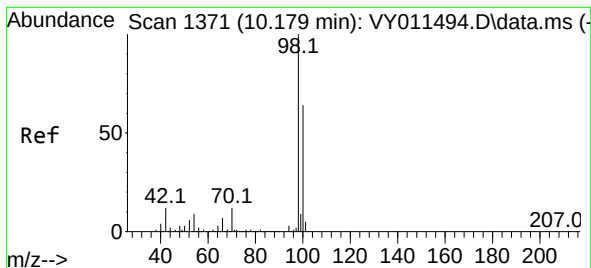

#50
Toluene-d8
Concen: 54.667 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY011541.D
Acq: 22 Nov 2022 12:30




Instrument : MSVOA_Y
ClientSampleId : BANK-RUN-SOIL-SAMPLE-3


Tgt Ion: 98 Resp: 334324
Ion Ratio Lower Upper
98 100
100 63.6 50.2 75.2

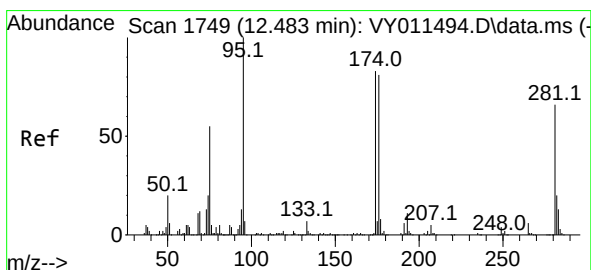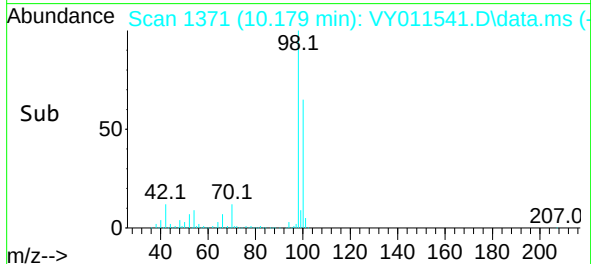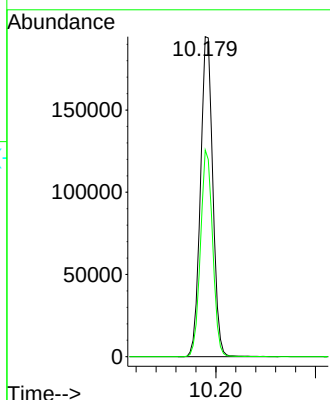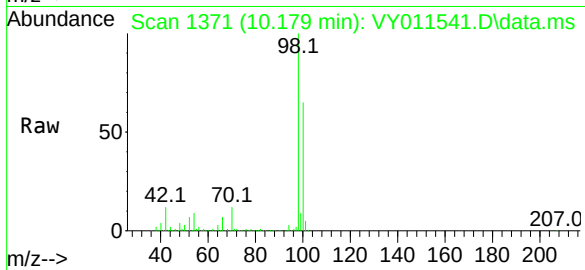

#62
4-Bromofluorobenzene
Concen: 43.571 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY011541.D
Acq: 22 Nov 2022 12:30

Tgt Ion: 95 Resp: 98520
Ion Ratio Lower Upper
95 100
174 84.5 0.0 177.0
176 79.9 0.0 175.8


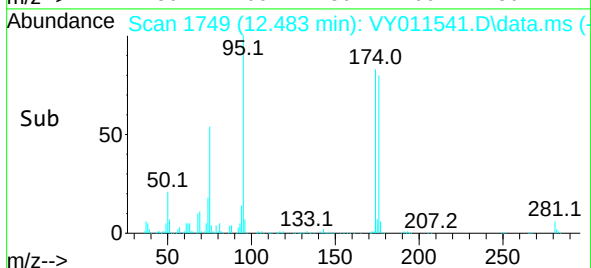
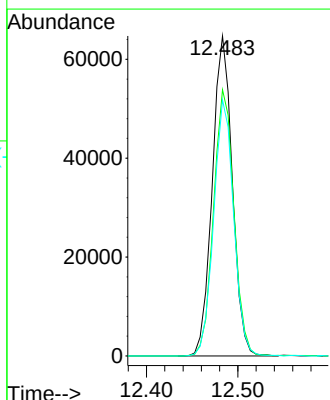
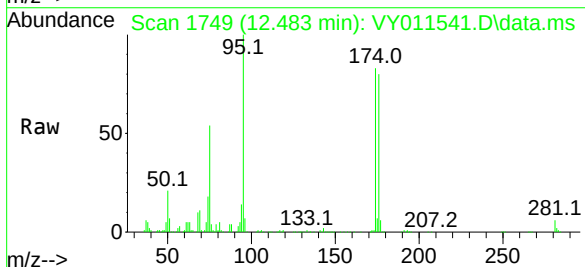


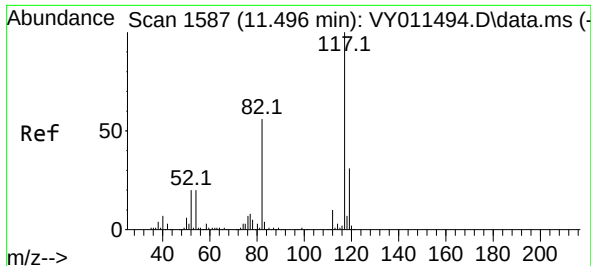

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11586
Delta R.T. -0.007 min
Lab File: VY011541.D
Acq: 22 Nov 2022 12:30

Instrument :
MSVOA_Y
ClientSampleId :
BANK-RUN-SOIL-SAMPLE-3

Tgt Ion:117 Resp: 249863
Ion Ratio Lower Upper
117 100
82 57.8 43.0 64.4
119 32.3 25.4 38.0

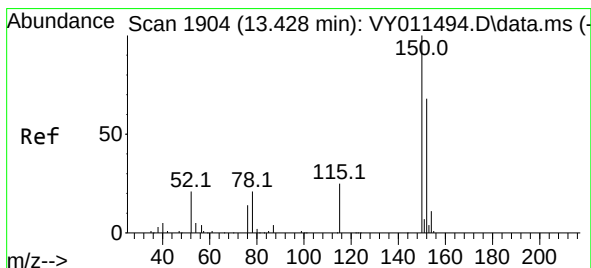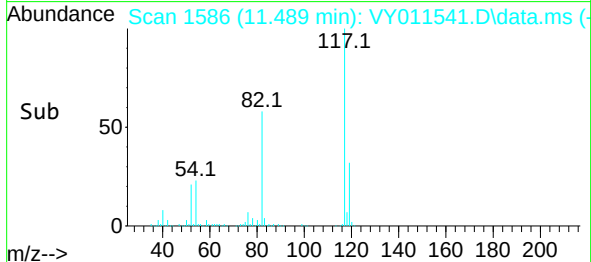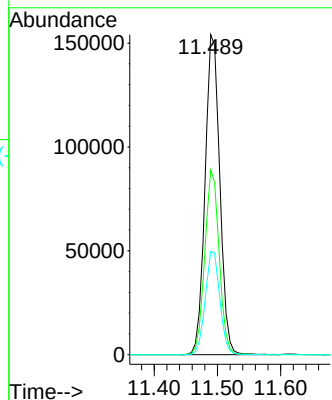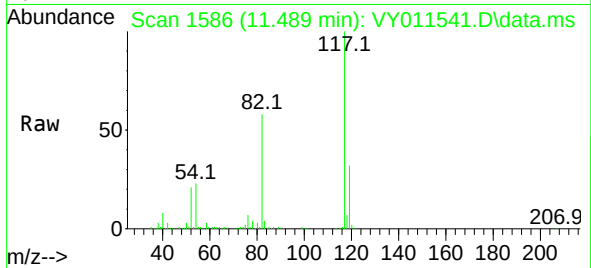

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY011541.D
Acq: 22 Nov 2022 12:30

Tgt Ion:152 Resp: 101067
Ion Ratio Lower Upper
152 100
115 58.4 28.2 84.7
150 157.0 0.0 347.6

