

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112222\
 Data File : VY011552.D
 Acq On : 22 Nov 2022 16:48
 Operator : KP/MD
 Sample : N5718-03RE
 Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VNJ-228RE

Quant Time: Nov 23 04:08:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111822S.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 19 22:37:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	2722	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	4136	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	3740	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	754	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	2068	74.822	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	149.640%
35) Dibromofluoromethane	7.716	113	876	34.406	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	68.820%
50) Toluene-d8	10.179	98	5176	55.943	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	111.880%
62) 4-Bromofluorobenzene	12.483	95	1097	32.068	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	64.140%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112222\
Data File : VY011552.D
Acq On : 22 Nov 2022 16:48
Operator : KP/MD
Sample : N5718-03RE
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VNJ-228RE

Quant Time: Nov 23 04:08:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111822S.M
Quant Title : SW846 8260
QLast Update : Sat Nov 19 22:37:14 2022
Response via : Initial Calibration




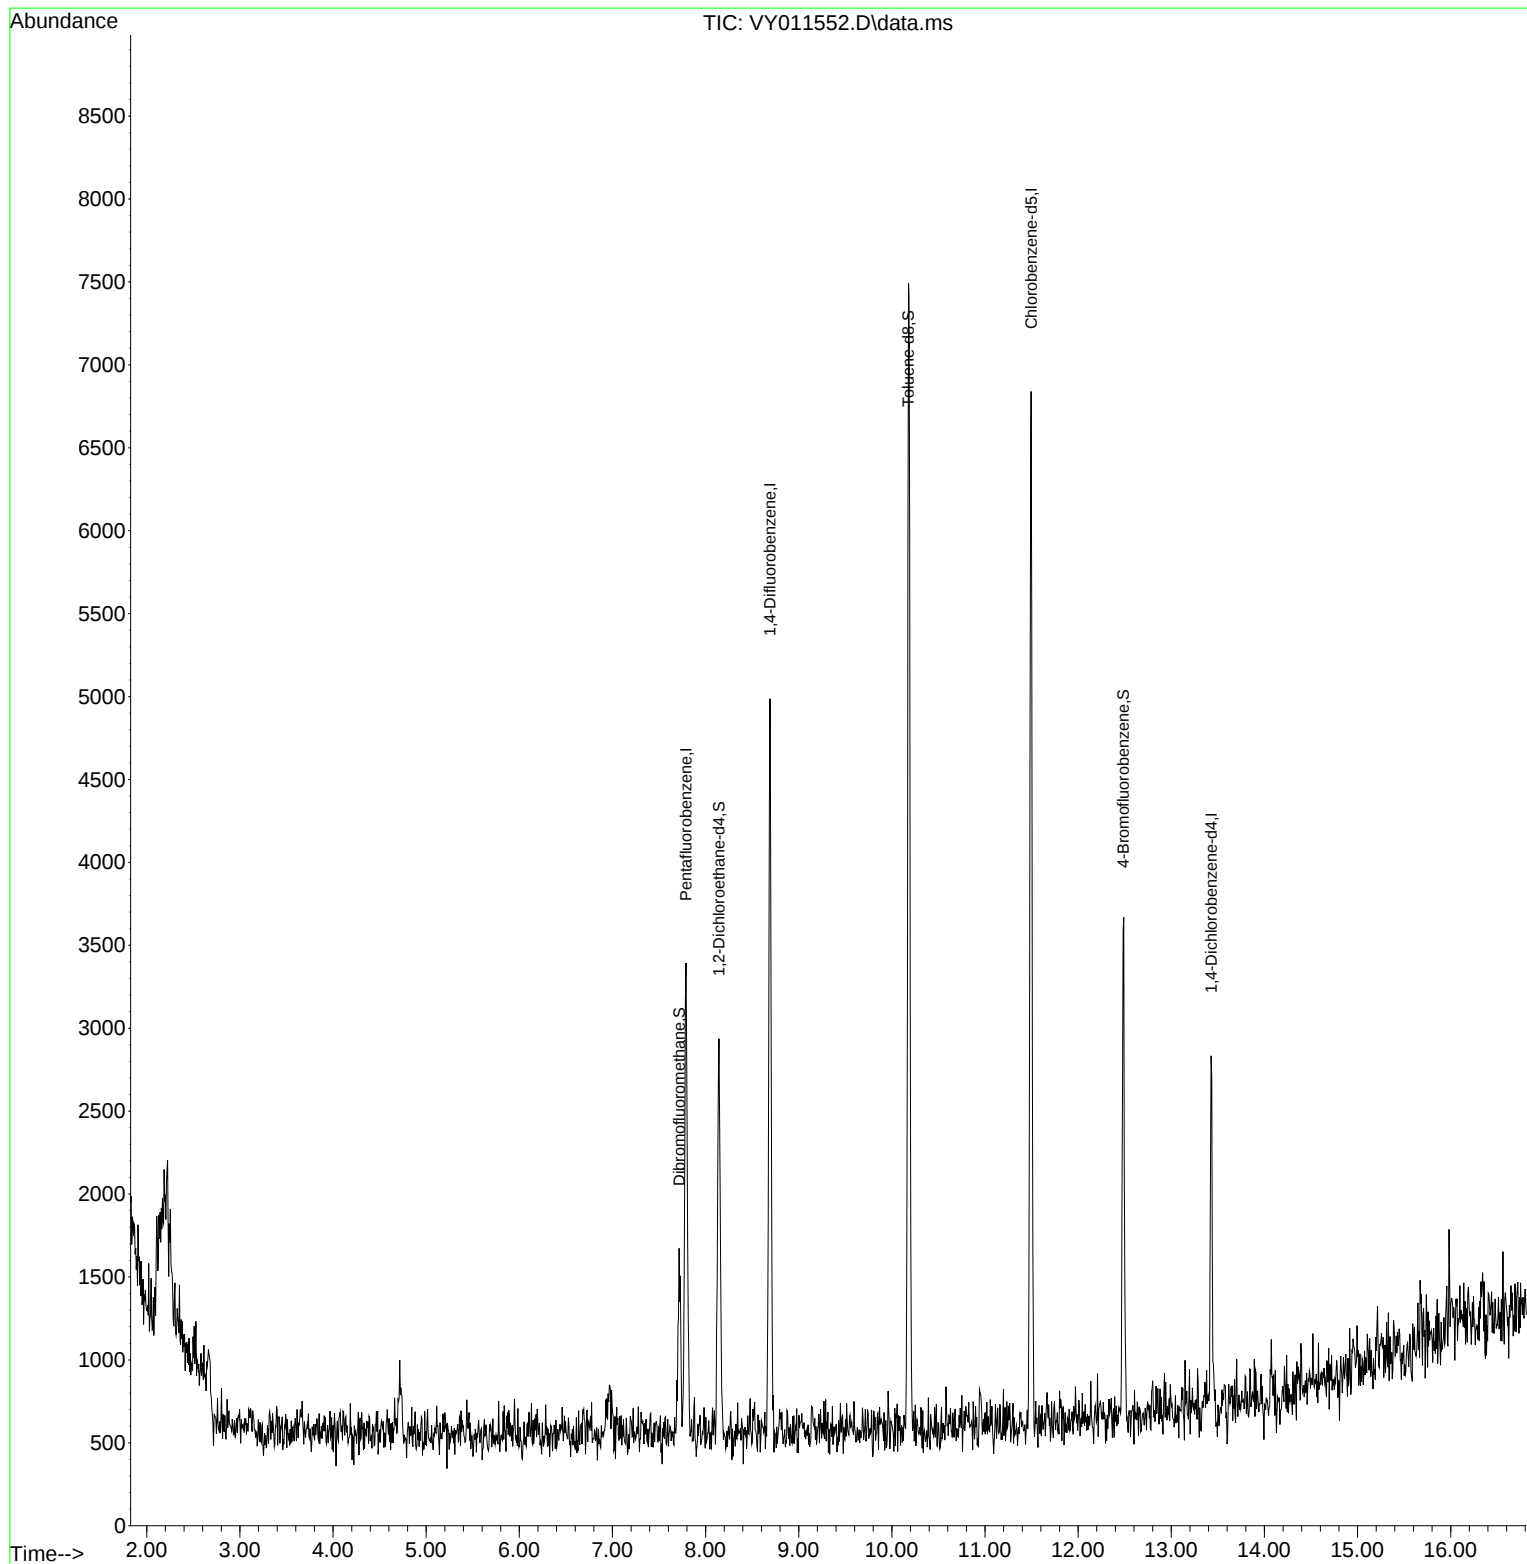


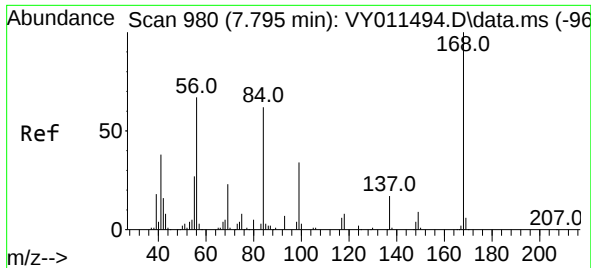

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY011552.D
Acq: 22 Nov 2022 16:48




Instrument :
MSVOA_Y
ClientSampleId :
VNJ-228RE

Tgt Ion:168 Resp: 2722
Ion Ratio Lower Upper
168 100
99 53.4 46.9 70.3

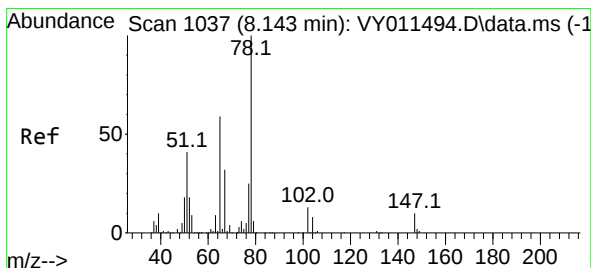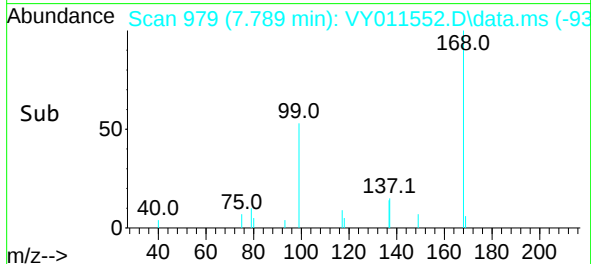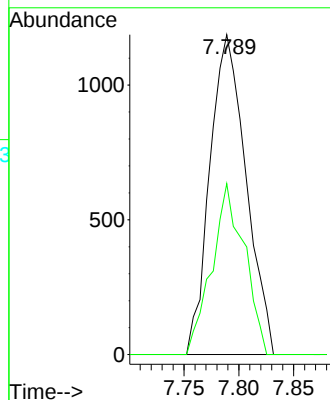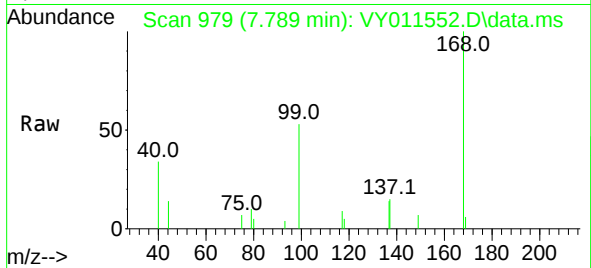

#33
1,2-Dichloroethane-d4
Concen: 74.822 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. -0.001 min
Lab File: VY011552.D
Acq: 22 Nov 2022 16:48

Tgt Ion: 65 Resp: 2068
Ion Ratio Lower Upper
65 100
67 45.8 0.0 99.4


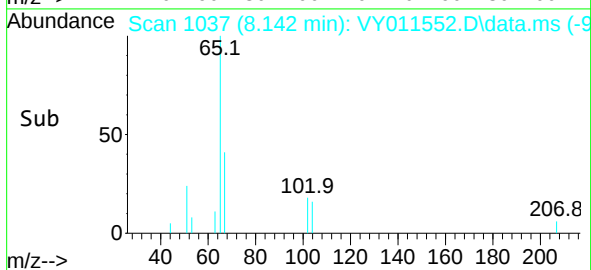
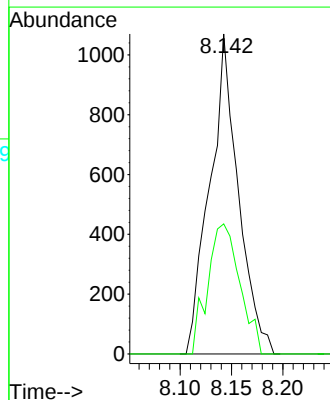
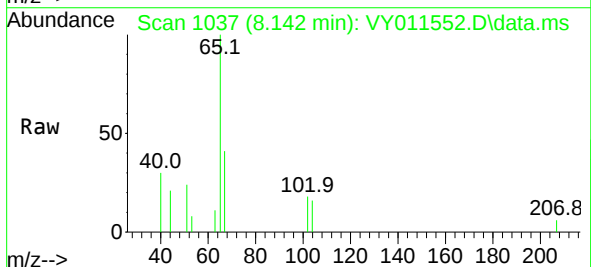




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VY011552.D
Acq: 22 Nov 2022 16:48




Instrument :
MSVOA_Y
ClientSampleId :
VNJ-228RE


Tgt Ion:	114	Resp:	4136
Ion	Ratio	Lower	Upper
114	100		
63	15.7	0.0	43.2
88	17.6	0.0	31.8

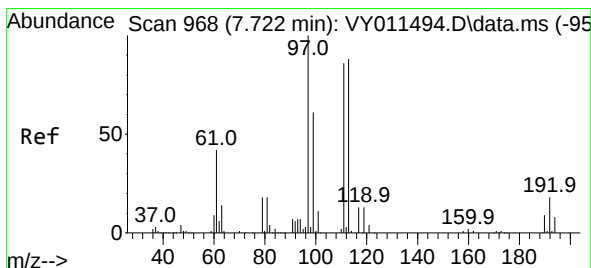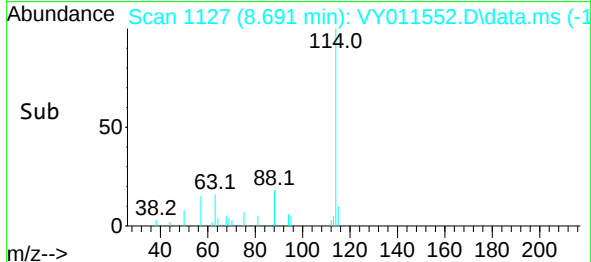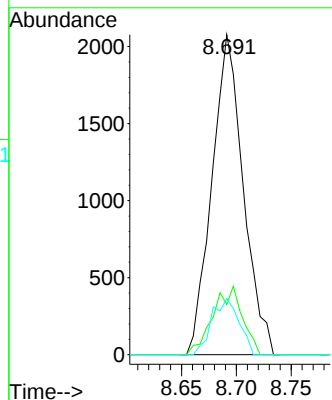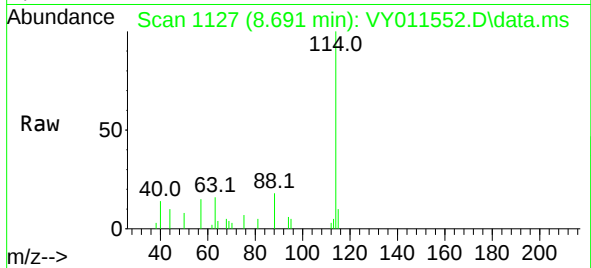

#35
Dibromofluoromethane
Concen: 34.406 ug/l
RT: 7.716 min Scan# 967
Delta R.T. -0.006 min
Lab File: VY011552.D
Acq: 22 Nov 2022 16:48

Tgt Ion:	113	Resp:	876
Ion	Ratio	Lower	Upper
113	100		
111	89.8	82.6	124.0
192	14.5	17.6	26.4

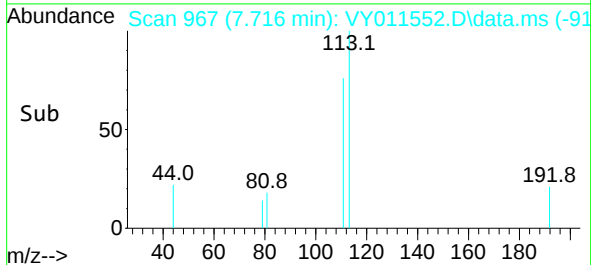
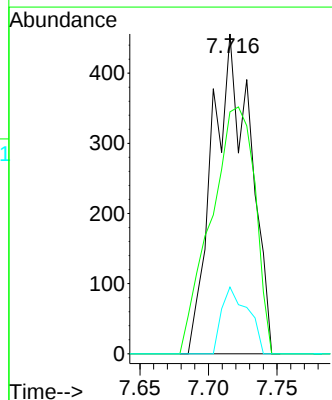
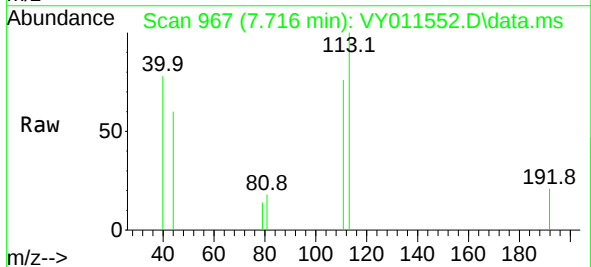


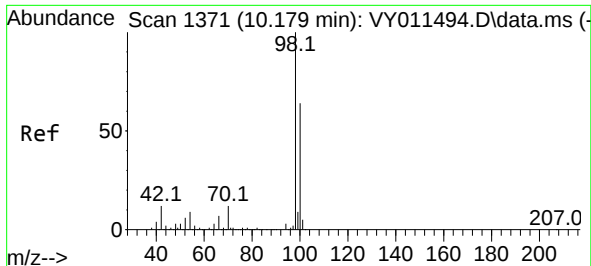

#50
Toluene-d8
Concen: 55.943 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY011552.D
Acq: 22 Nov 2022 16:48




Instrument :
MSVOA_Y
ClientSampleId :
VNJ-228RE

Tgt Ion: 98 Resp: 5176
Ion Ratio Lower Upper
98 100
100 64.2 50.2 75.2

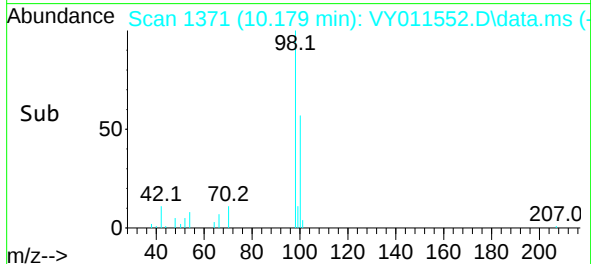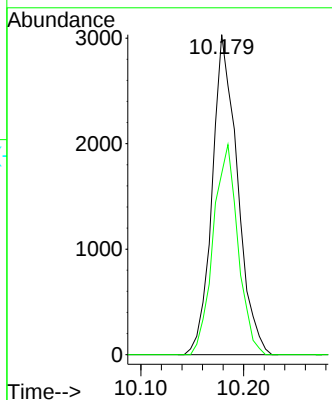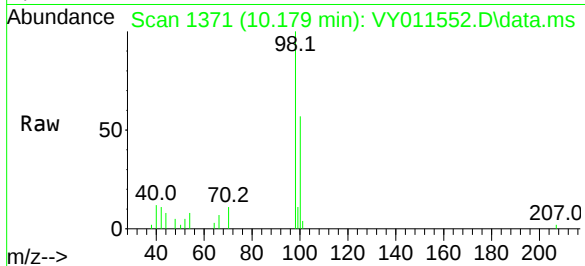

#62
4-Bromofluorobenzene
Concen: 32.068 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY011552.D
Acq: 22 Nov 2022 16:48

Tgt Ion: 95 Resp: 1097
Ion Ratio Lower Upper
95 100
174 89.4 0.0 177.0
176 77.2 0.0 175.8


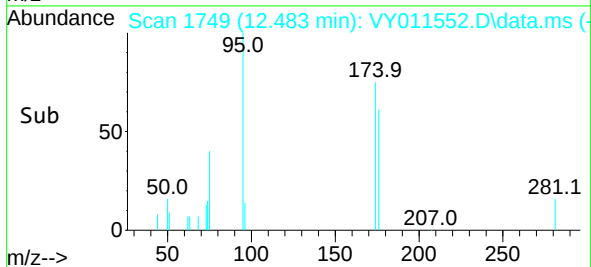
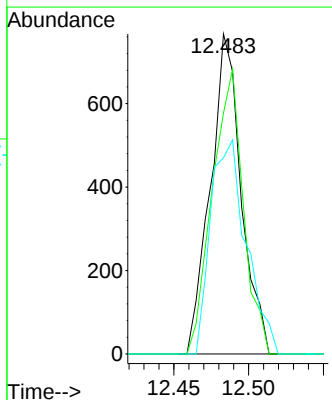
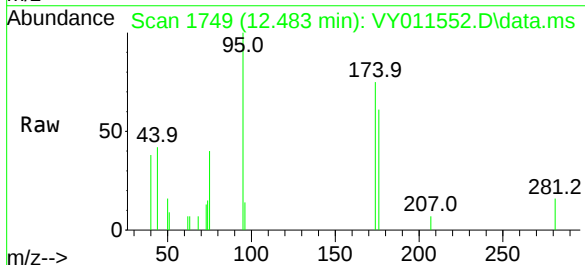




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.496 min Scan# 117
Delta R.T. -0.000 min
Lab File: VY011552.D
Acq: 22 Nov 2022 16:48

Instrument :
MSVOA_Y
ClientSampleId :
VNJ-228RE

Tgt Ion:117 Resp: 3740
Ion Ratio Lower Upper
117 100
82 45.9 43.0 64.4
119 30.4 25.4 38.0

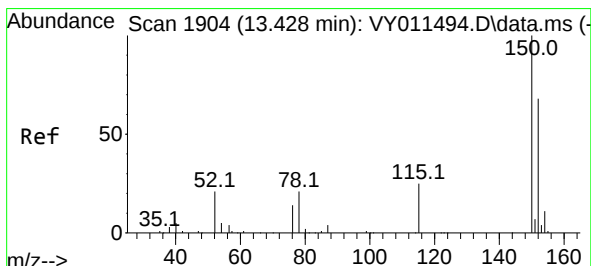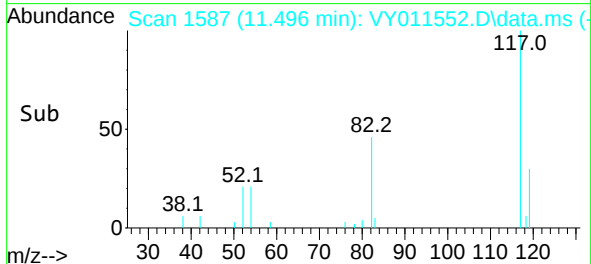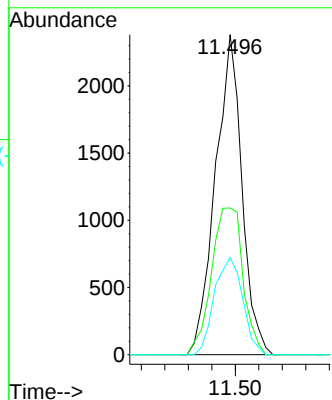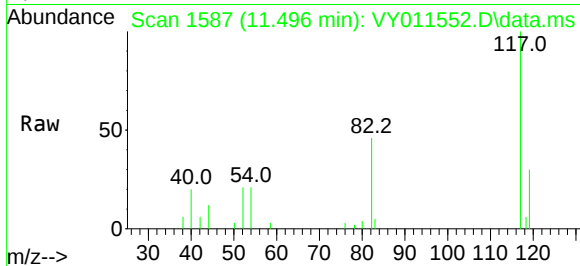

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY011552.D
Acq: 22 Nov 2022 16:48

Tgt Ion:152 Resp: 754
Ion Ratio Lower Upper
152 100
115 48.7 28.2 84.7
150 148.3 0.0 347.6

