
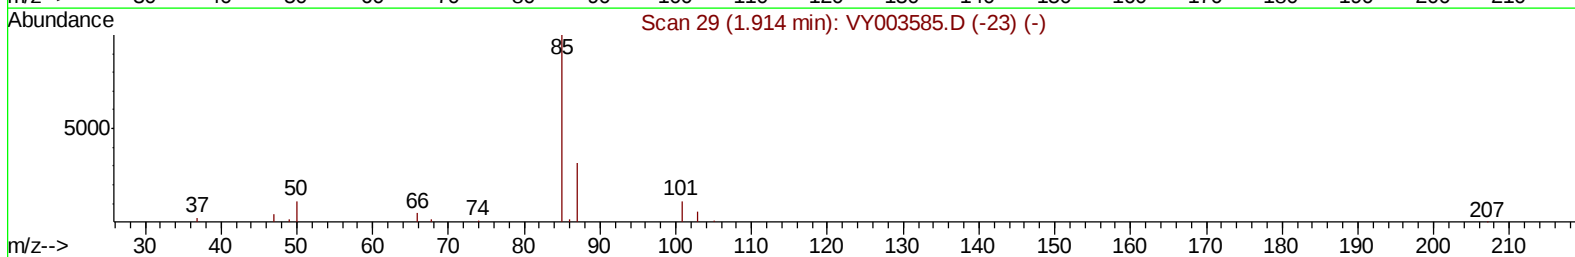
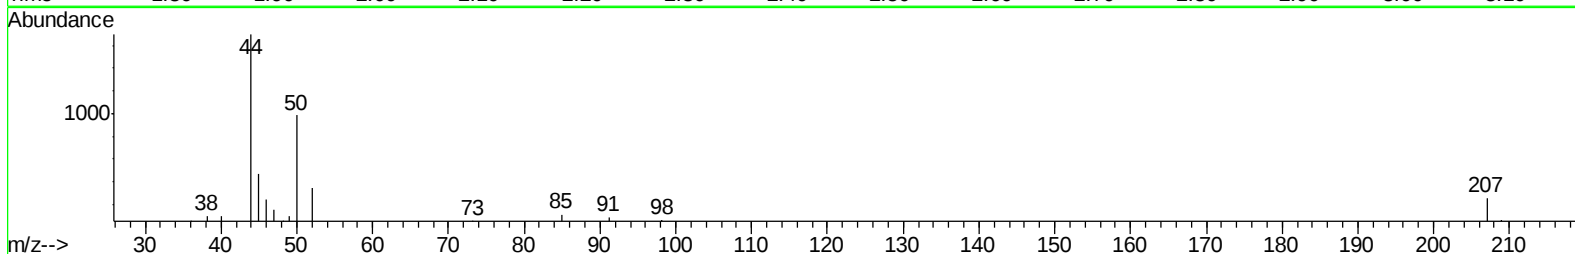


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\VY112320\
Data File : VY003591.D
Acq On : 23 Nov 2020 15:19
Operator : SY/MD
Sample : L4824-06
Misc : 5.00G/10ML/MSVOA Y/SOIL
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 03 08:58:50 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SFAMYLEM112320SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 24 14:47:44 2020
Response via : Initial Calibration

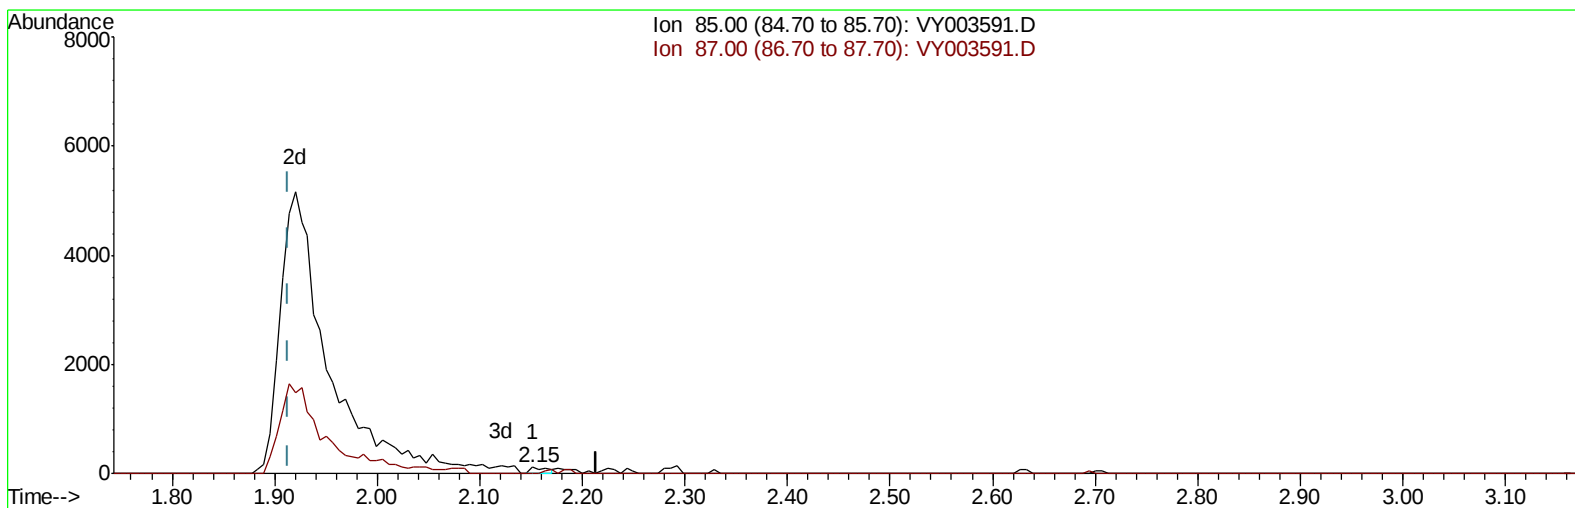

TIC: VY003591.D

(2) Dichlorodifluoromethane (T)




2.152min (+0.238) 0.11ug/L

response 128

Ion	Exp%	Act%
85.00	100	100
87.00	34.00	35.16
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\VY112320\
Data File : VY003591.D
Acq On : 23 Nov 2020 15:19
Operator : SY/MD
Sample : L4824-06
Misc : 5.00G/10ML/MSVOA Y/SOIL
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 03 08:58:50 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SFAMYL112320SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 24 14:47:44 2020
Response via : Initial Calibration

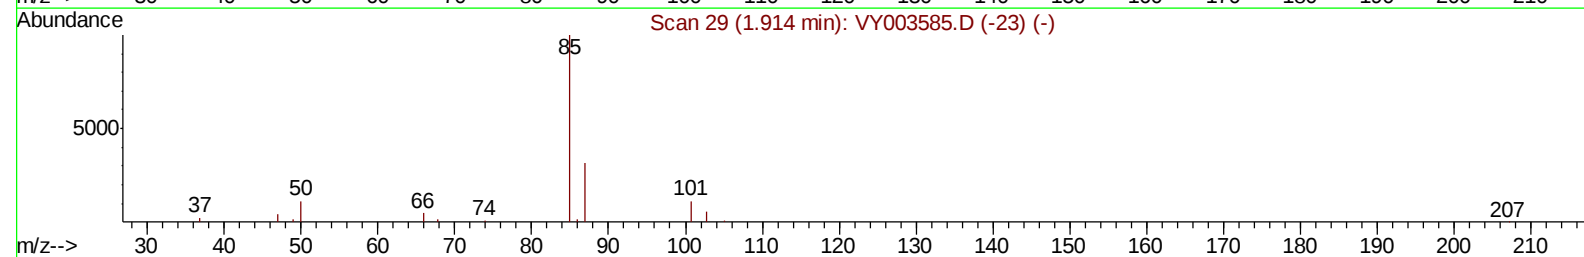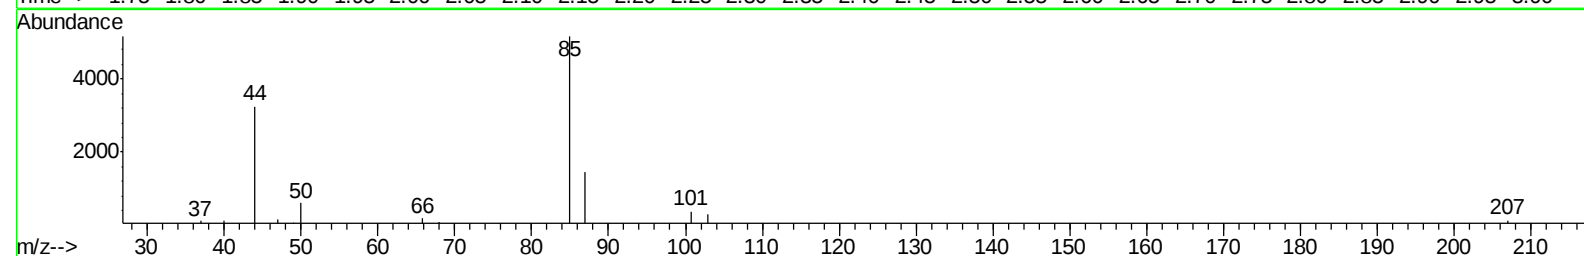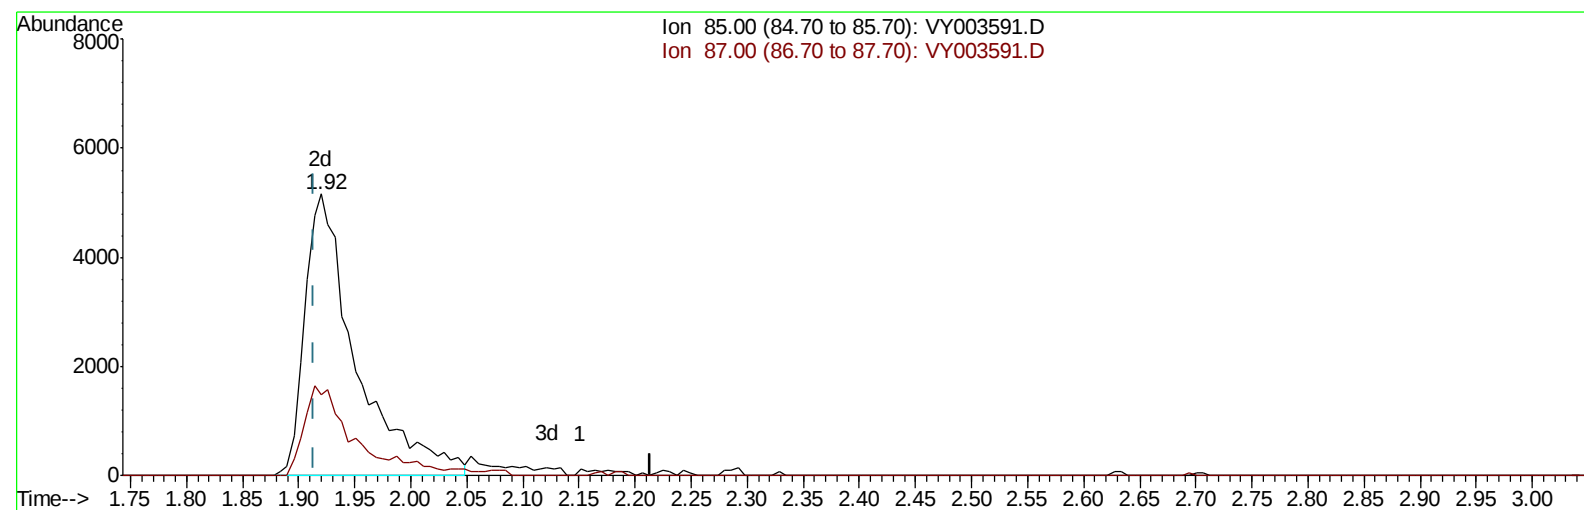

TIC: VY003591.D

(2) Dichlorodifluoromethane (T)

1.920min (+0.006) 13.67ug/L m

response 16305

Ion	Exp%	Act%
85.00	100	100
87.00	34.00	0.28#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\VY112320\
 Data File : VY003591.D
 Acq On : 23 Nov 2020 15:19
 Operator : SY/MD
 Sample : L4824-06
 Misc : 5.00G/10ML/MSVOA Y/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 03 09:10:56 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SFAMYL112320SMA.M

Quant Title : VOC Analysis

QLast Update : Tue Nov 24 14:47:44 2020

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.69	114	223082	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.49	117	203311	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.42	152	105040	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.25	65	75317	23.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.72%
7) Chloroethane-d5	2.77	69	63413	24.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.20%
11) 1,1-Dichloroethene-d2	3.85	63	146243	21.92	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	87.68%
21) 2-Butanone-d5	6.90	46	67100	49.83	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.66%
24) Chloroform-d	7.48	84	152789	24.21	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.84%
26) 1,2-Dichloroethane-d4	8.14	65	85477	24.48	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.92%
32) Benzene-d6	8.11	84	321052	24.82	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.28%
36) 1,2-Dichloropropane-d6	9.12	67	96389	24.52	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.08%
41) Toluene-d8	10.17	98	282293	24.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.36%
43) trans-1,3-Dichloropropene-	10.44	79	46343	24.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	99.40%
47) 2-Hexanone-d5	10.78	63	51162	51.24	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.48%
56) 1,1,2,2-Tetrachloroethane-	12.56	84	85170	25.08	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.32%
66) 1,2-Dichlorobenzene-d4	13.72	152	90760	24.92	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.68%

Target Compounds

					Ovalue
2) Dichlorodifluoromethane	1.92	85	16305m	13.671	ug/L
3) Chloromethane	2.12	50	31161	13.809	ug/L
5) Vinyl chloride	2.26	62	82907	26.079	ug/L
6) Bromomethane	2.66	94	34575	14.857	ug/L
8) Chloroethane	2.80	64	19018	9.569	ug/L
9) Trichlorofluoromethane	3.13	101	23796	10.252	ug/L
10) 1,1,2-Trichloro-1,2,2-trif	3.90	101	65382	21.474	ug/L
12) 1,1-Dichloroethene	3.88	96	51389	15.869	ug/L
15) Methyl Acetate	4.48	43	57522	24.108	ug/L
16) Methylene chloride	4.72	84	79501	18.223	ug/L
18) Methyl tert-butyl Ether	5.22	73	209202	41.005	ug/L
22) 2-Butanone	6.99	43	150011	98.350	ug/L
25) Chloroform	7.50	83	115398	19.927	ug/L
29) Cyclohexane	7.78	56	103671	20.762	ug/L
33) Benzene	8.16	78	550028	41.224	ug/L
34) Trichloroethene	8.94	95	175375	53.014	ug/L
42) Toluene	10.24	91	713937	50.928	ug/L

Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\VY112320\
 Data File : VY003591.D
 Acq On : 23 Nov 2020 15:19
 Operator : SY/MD
 Sample : L4824-06
 Misc : 5.00G/10ML/MSVOA Y/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 03 09:10:56 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SFAMYL112320SMA.M

Quant Title : VOC Analysis

QLast Update : Tue Nov 24 14:47:44 2020

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
45) 1,1,2-Trichloroethane	10.64	97	54150	19.805	ug/L	97
46) Tetrachloroethene	10.72	164	29864	10.301	ug/L	98
51) Chlorobenzene	11.51	112	114582	12.846	ug/L	99
52) Ethylbenzene	11.59	91	367033	25.660	ug/L	98
53) m,p-Xylene	11.70	106	175946	31.873	ug/L	95
54) o-Xylene	12.03	106	121594	26.062	ug/L	97
55) Styrene	12.04	104	99876	10.946	ug/L	97
57) 1,1,2,2-Tetrachloroethane	12.58	83	39760	12.079	ug/L #	95
59) Bromoform	12.20	173	25902	11.592	ug/L	97
60) Isopropylbenzene	12.33	105	213759	20.164	ug/L	100
63) 1,2,4-Trimethylbenzene	13.12	105	210160	25.428	ug/L	100
64) 1,3-Dichlorobenzene	13.36	146	137596	20.436	ug/L	98
65) 1,4-Dichlorobenzene	13.44	146	70223	10.017	ug/L	98
70) 1,2,4-trichlorobenzene	15.00	180	61958	19.717	ug/L	98
72) 1,2,3-Trichlorobenzene	15.42	180	74021	31.168	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\VY112320\
Data File : VY003591.D
Acq On : 23 Nov 2020 15:19
Operator : SY/MD
Sample : L4824-06
Misc : 5.00G/10ML/MSVOA Y/SOIL
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 03 09:10:56 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\SFAMYL112320SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 24 14:47:44 2020
Response via : Initial Calibration

