

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112524\
 Data File : VY020436.D
 Acq On : 25 Nov 2024 17:44
 Operator : SY/MD
 Sample : P4960-06
 Misc : 5.10g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SW4

Quant Time: Nov 26 00:47:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111924S.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 20 04:38:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	16447	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	22399	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	13787	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	2505	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.067	65	4476	23.688	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	47.380%#
35) Dibromofluoromethane	7.640	113	6106	42.512	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	85.020%
50) Toluene-d8	10.109	98	24372	43.076	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	86.160%
62) 4-Bromofluorobenzene	12.408	95	3817	20.986	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	41.980%


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112524\
Data File : VY020436.D
Acq On : 25 Nov 2024 17:44
Operator : SY/MD
Sample : P4960-06
Misc : 5.10g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SW4

Quant Time: Nov 26 00:47:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111924S.M
Quant Title : SW846 8260
QLast Update : Wed Nov 20 04:38:24 2024
Response via : Initial Calibration




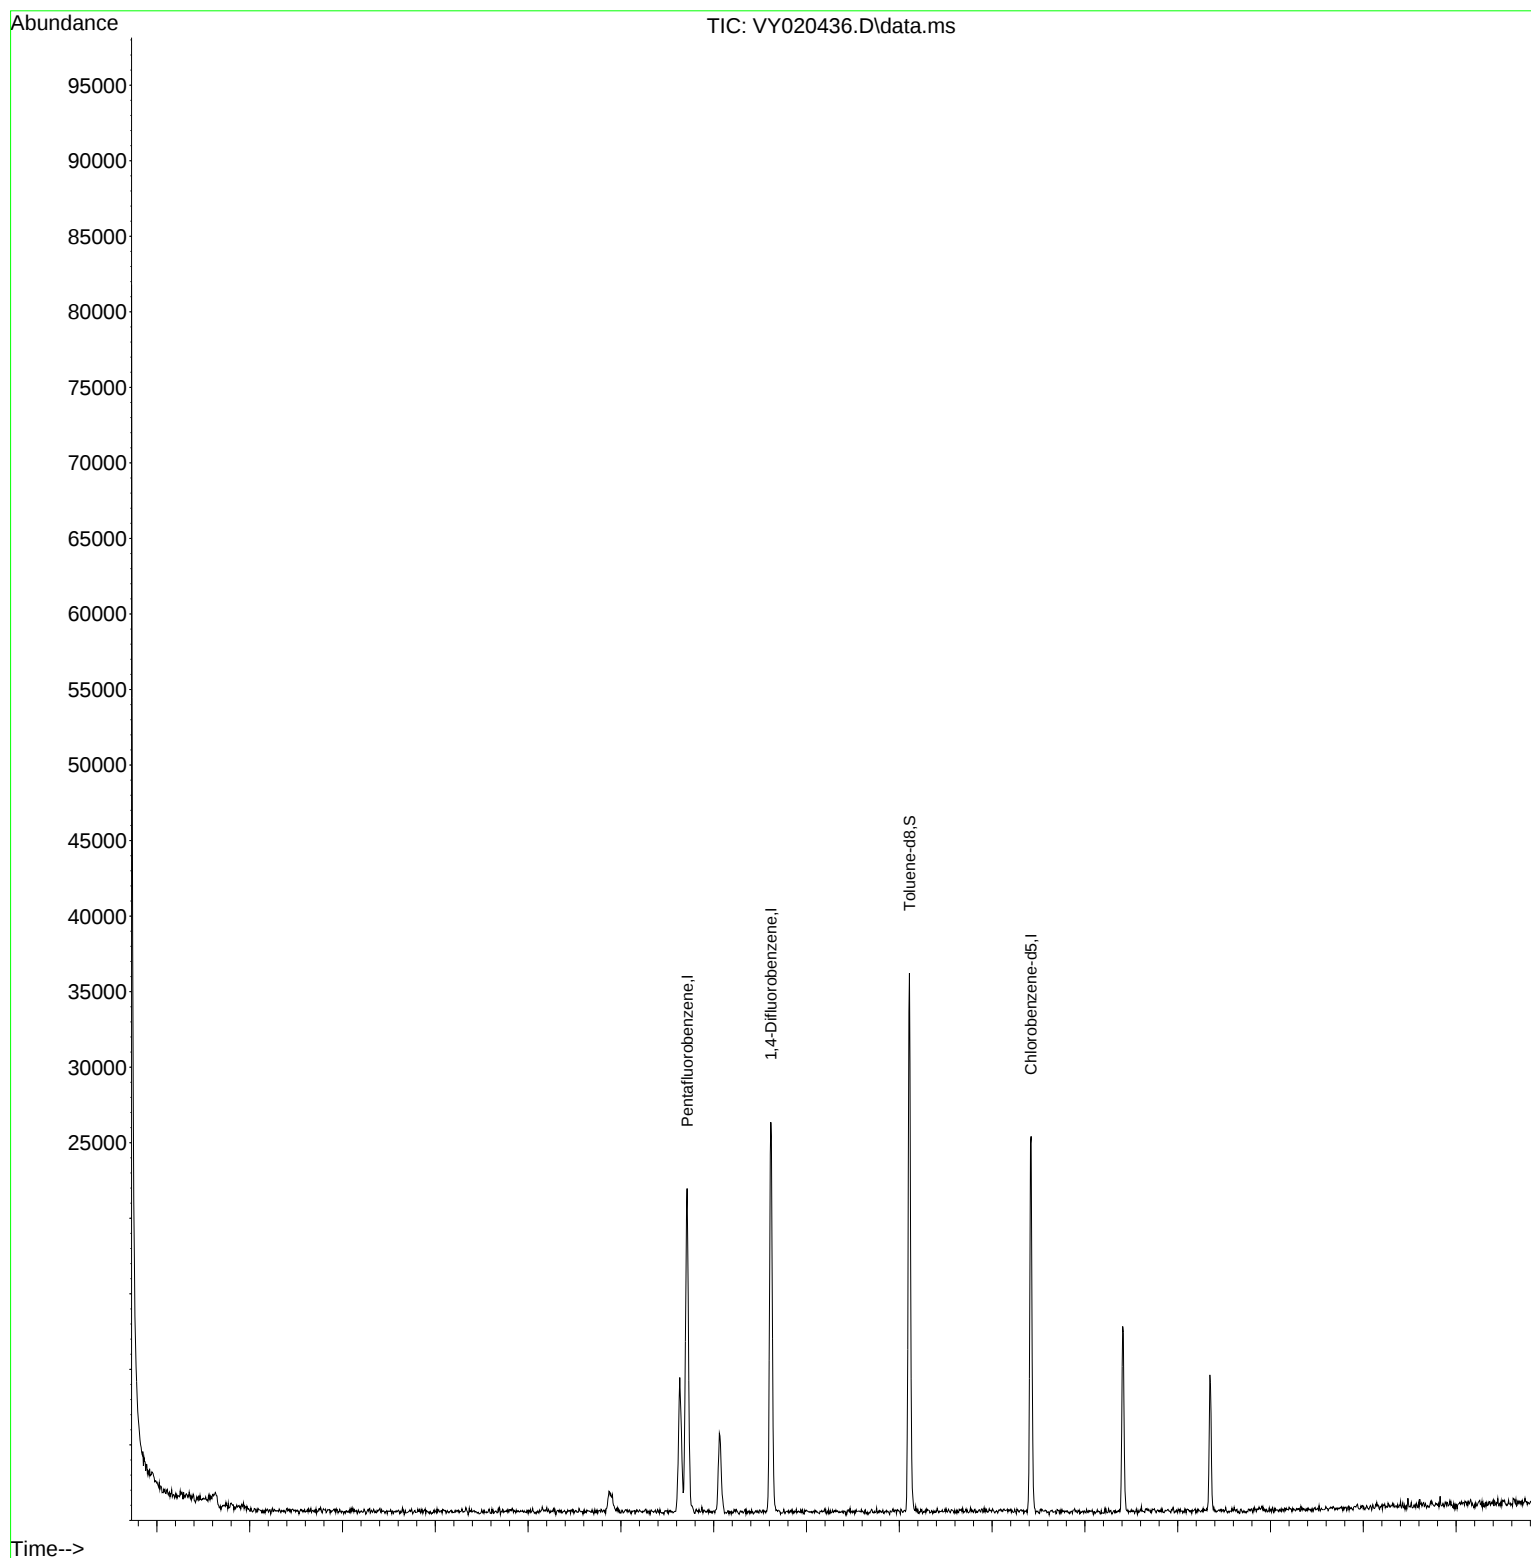


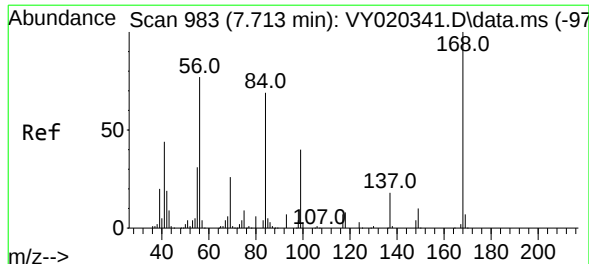

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 98
Delta R.T. 0.000 min
Lab File: VY020436.D
Acq: 25 Nov 2024 17:44




Instrument :
MSVOA_Y
ClientSampleId :
SW4


Tgt Ion:168 Resp: 16447
Ion Ratio Lower Upper
168 100
99 58.2 46.6 69.8

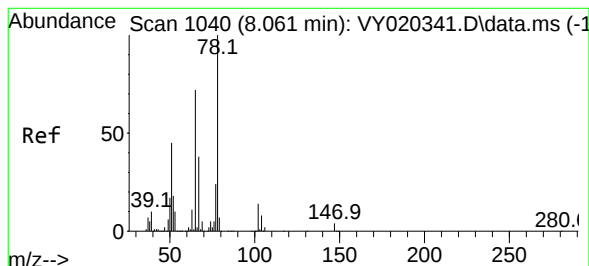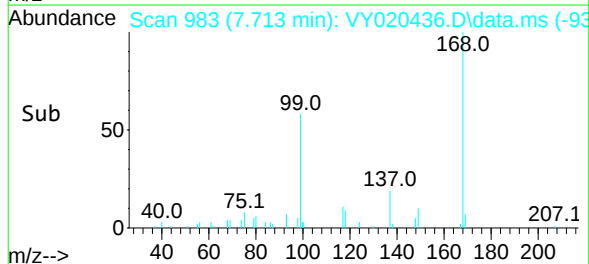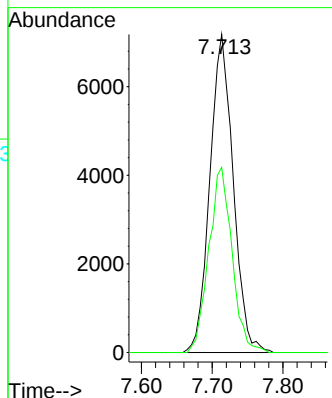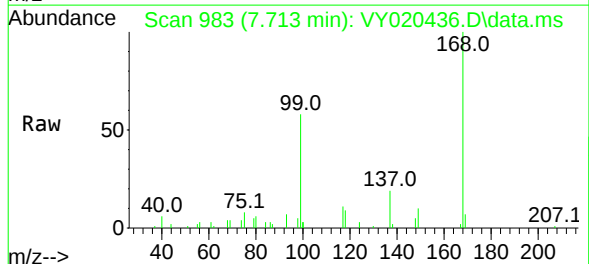

#33
1,2-Dichloroethane-d4
Concen: 23.688 ug/l
RT: 8.067 min Scan# 1041
Delta R.T. 0.006 min
Lab File: VY020436.D
Acq: 25 Nov 2024 17:44

Tgt Ion: 65 Resp: 4476
Ion Ratio Lower Upper
65 100
67 50.8 0.0 105.8


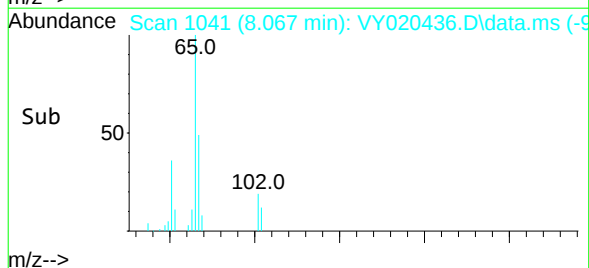
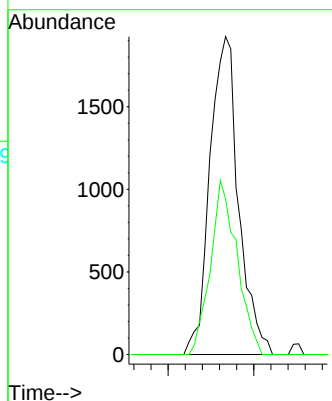
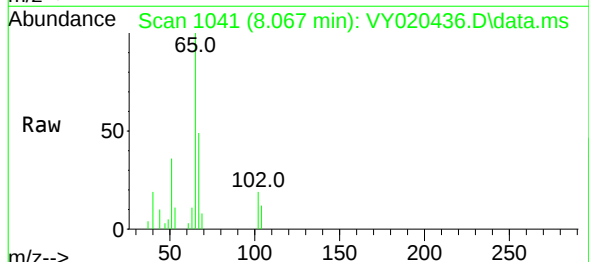


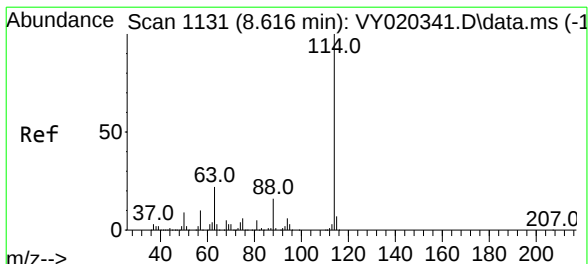

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.616 min Scan# 1131
 Delta R.T. 0.000 min
 Lab File: VY020436.D
 Acq: 25 Nov 2024 17:44




Instrument :
 MSVOA_Y
 ClientSampleId :
 SW4


Tgt Ion:	114	Resp:	22399
Ion	Ratio	Lower	Upper
114	100		
63	21.3	0.0	44.8
88	17.3	0.0	32.0

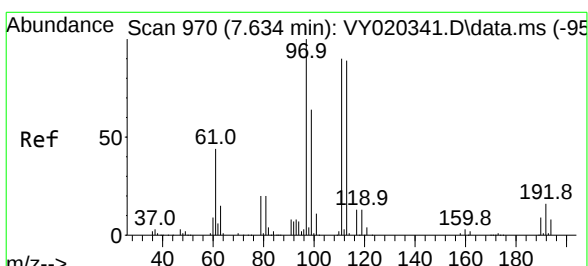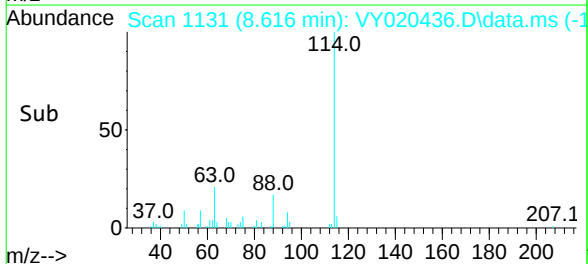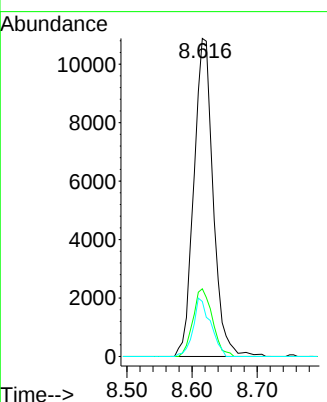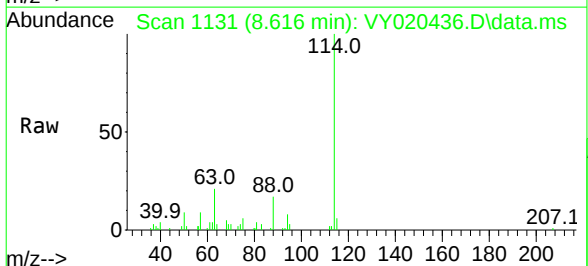

#35
 Dibromofluoromethane
 Concen: 42.512 ug/l
 RT: 7.640 min Scan# 971
 Delta R.T. 0.006 min
 Lab File: VY020436.D
 Acq: 25 Nov 2024 17:44

Tgt Ion:	113	Resp:	6106
Ion	Ratio	Lower	Upper
113	100		
111	105.0	81.4	122.0
192	18.8	15.1	22.7

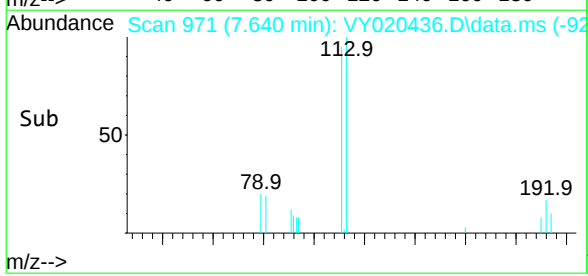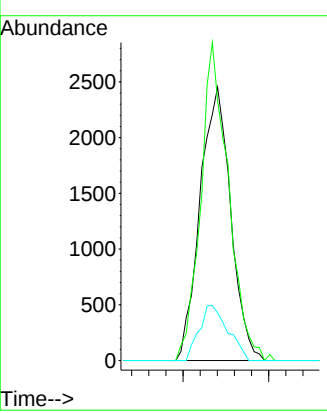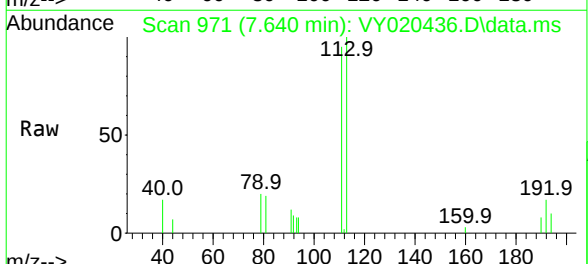

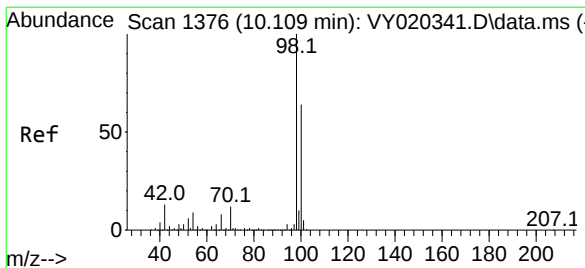

#50

Toluene-d8

Concen: 43.076 ug/l

RT: 10.109 min Scan# 1376

Delta R.T. 0.000 min

Lab File: VY020436.D

Acq: 25 Nov 2024 17:44

Instrument :

MSVOA_Y

ClientSampleId :





SW4

Tgt Ion: 98 Resp: 24372

Ion Ratio Lower Upper

98 100

100 62.5 51.3 76.9

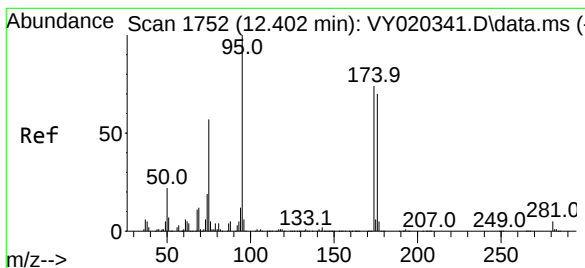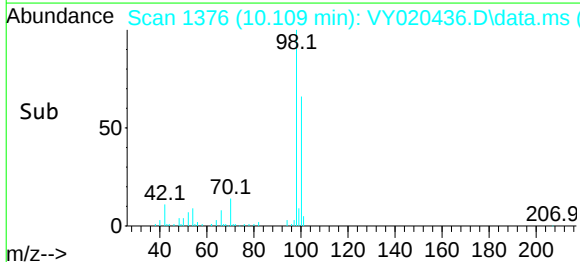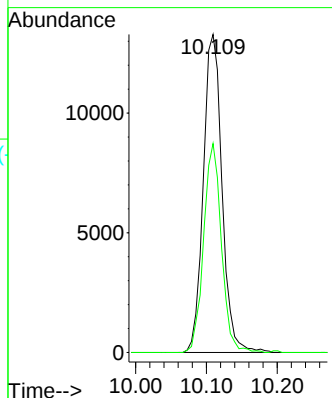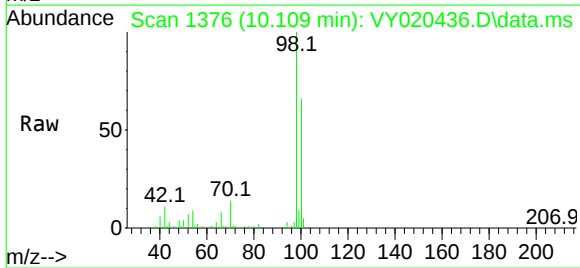

#62

4-Bromofluorobenzene

Concen: 20.986 ug/l

RT: 12.408 min Scan# 1753

Delta R.T. 0.006 min

Lab File: VY020436.D

Acq: 25 Nov 2024 17:44




Tgt Ion: 95 Resp: 3817


Ion Ratio Lower Upper

95 100

174 86.8 0.0 156.8

176 79.7 0.0 152.0

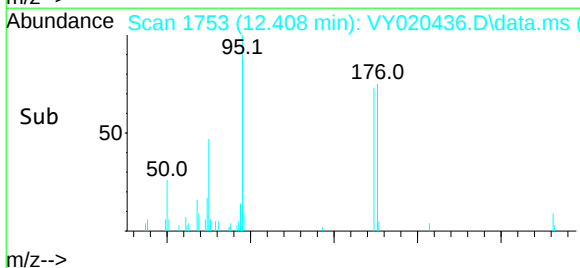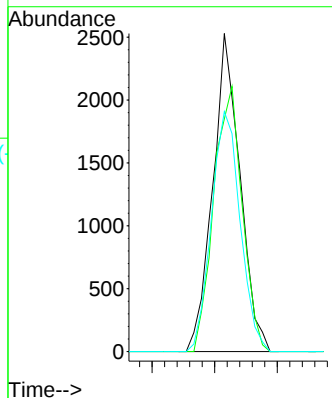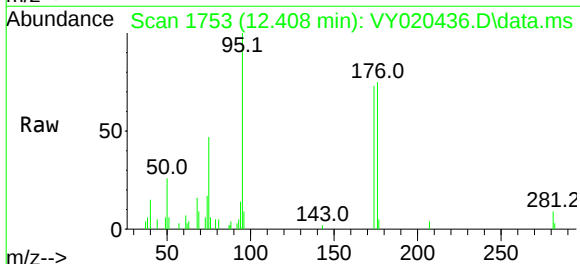

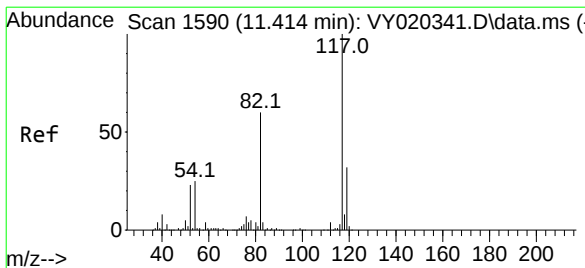

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.420 min Scan# 1591

Delta R.T. 0.006 min

Lab File: VY020436.D

Acq: 25 Nov 2024 17:44





Instrument :

MSVOA_Y

ClientSampleId :

SW4

Tgt Ion:	117	Resp:	13787
Ion Ratio	Lower	Upper	
117	100		
82	58.7	48.2	72.4
119	30.7	25.8	38.8

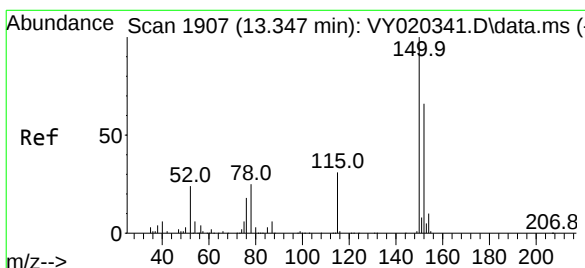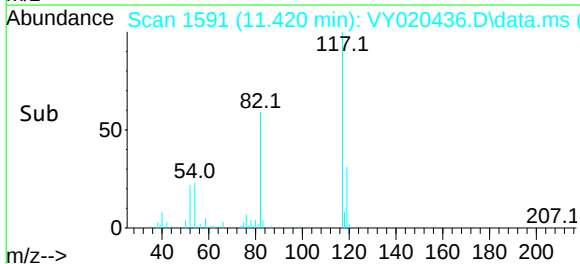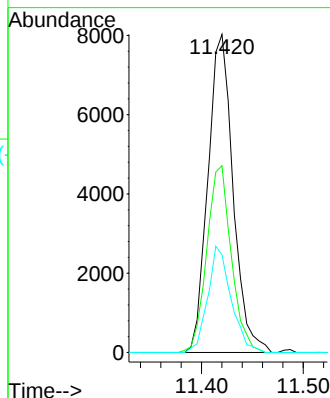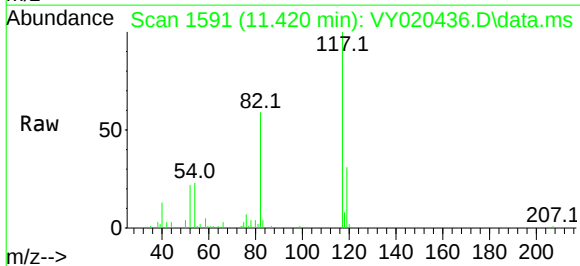

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY020436.D

Acq: 25 Nov 2024 17:44

Tgt Ion:	152	Resp:	2505
Ion Ratio	Lower	Upper	
152	100		
115	61.6	30.0	90.0
150	153.1	0.0	348.2

