



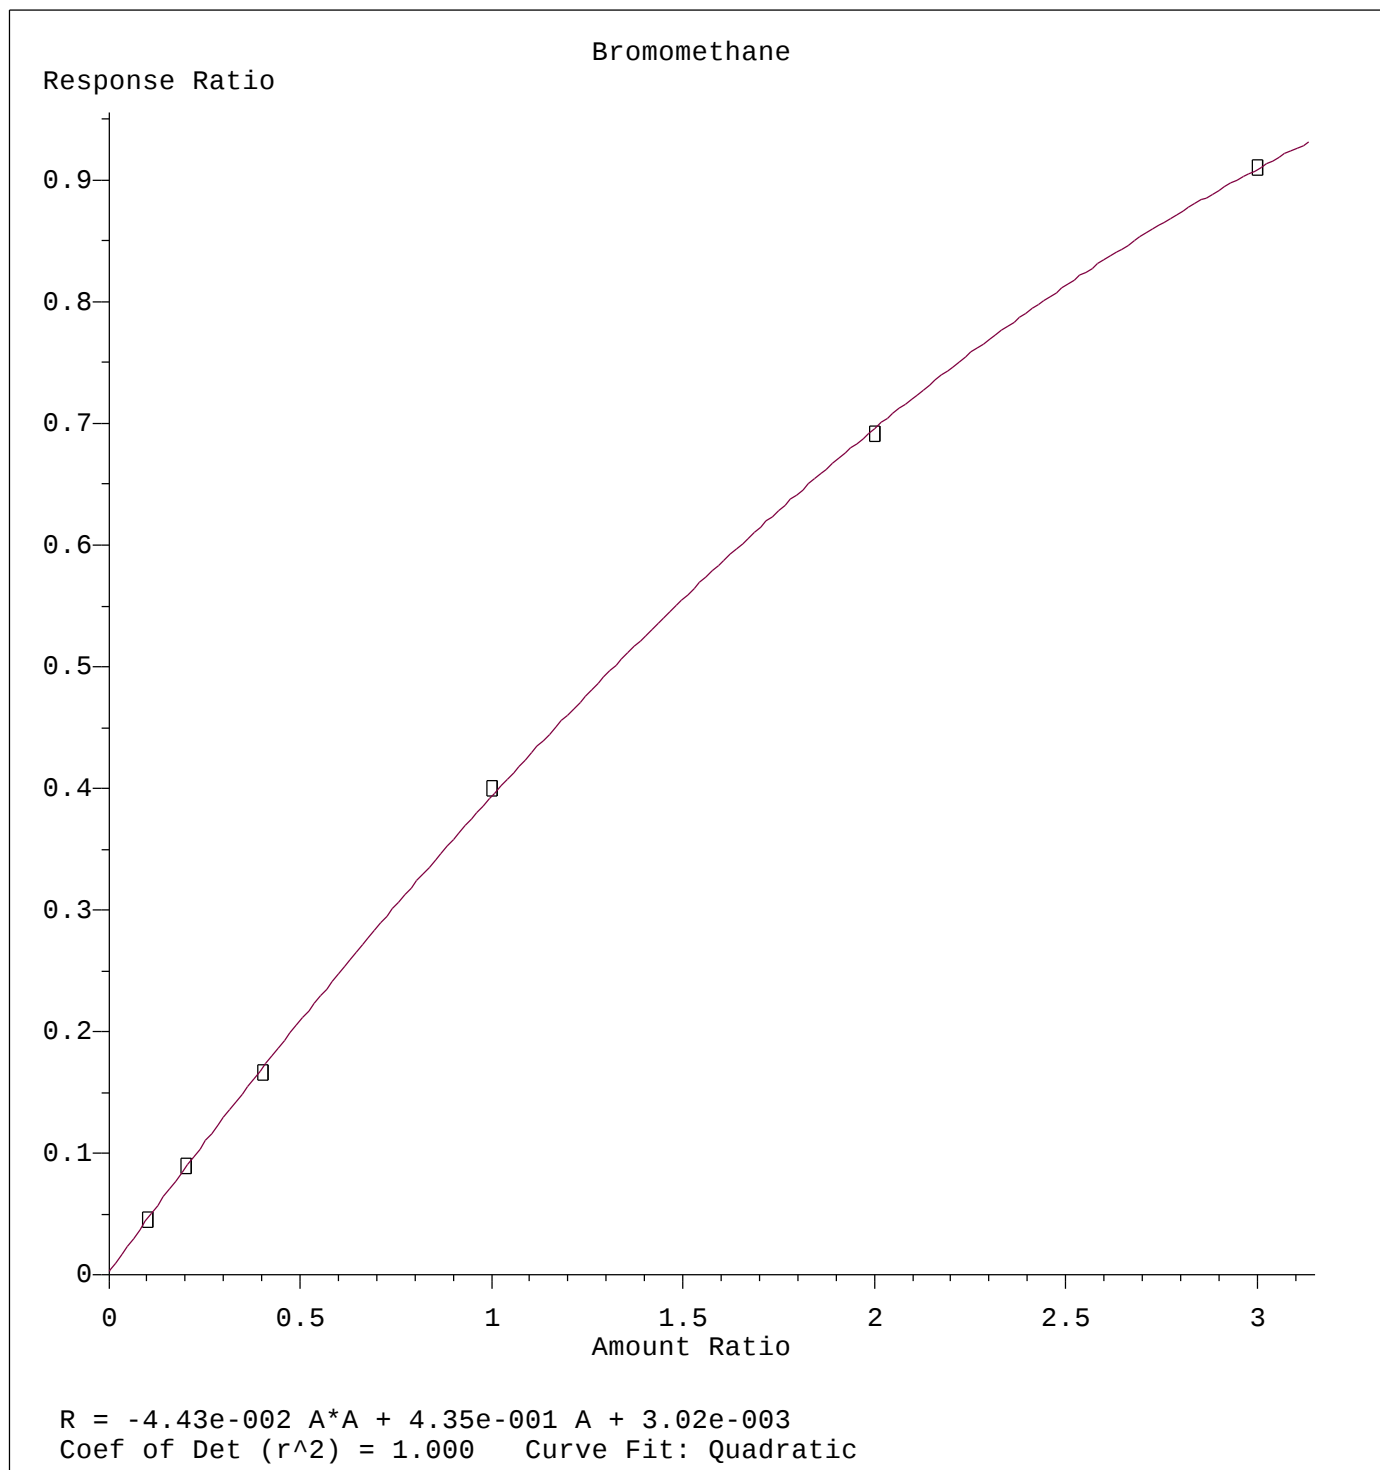

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y112719S.M
Calibration Table Last Updated: Wed Nov 27 12:40:47 2019

Bromochloromethane

Response Ratio

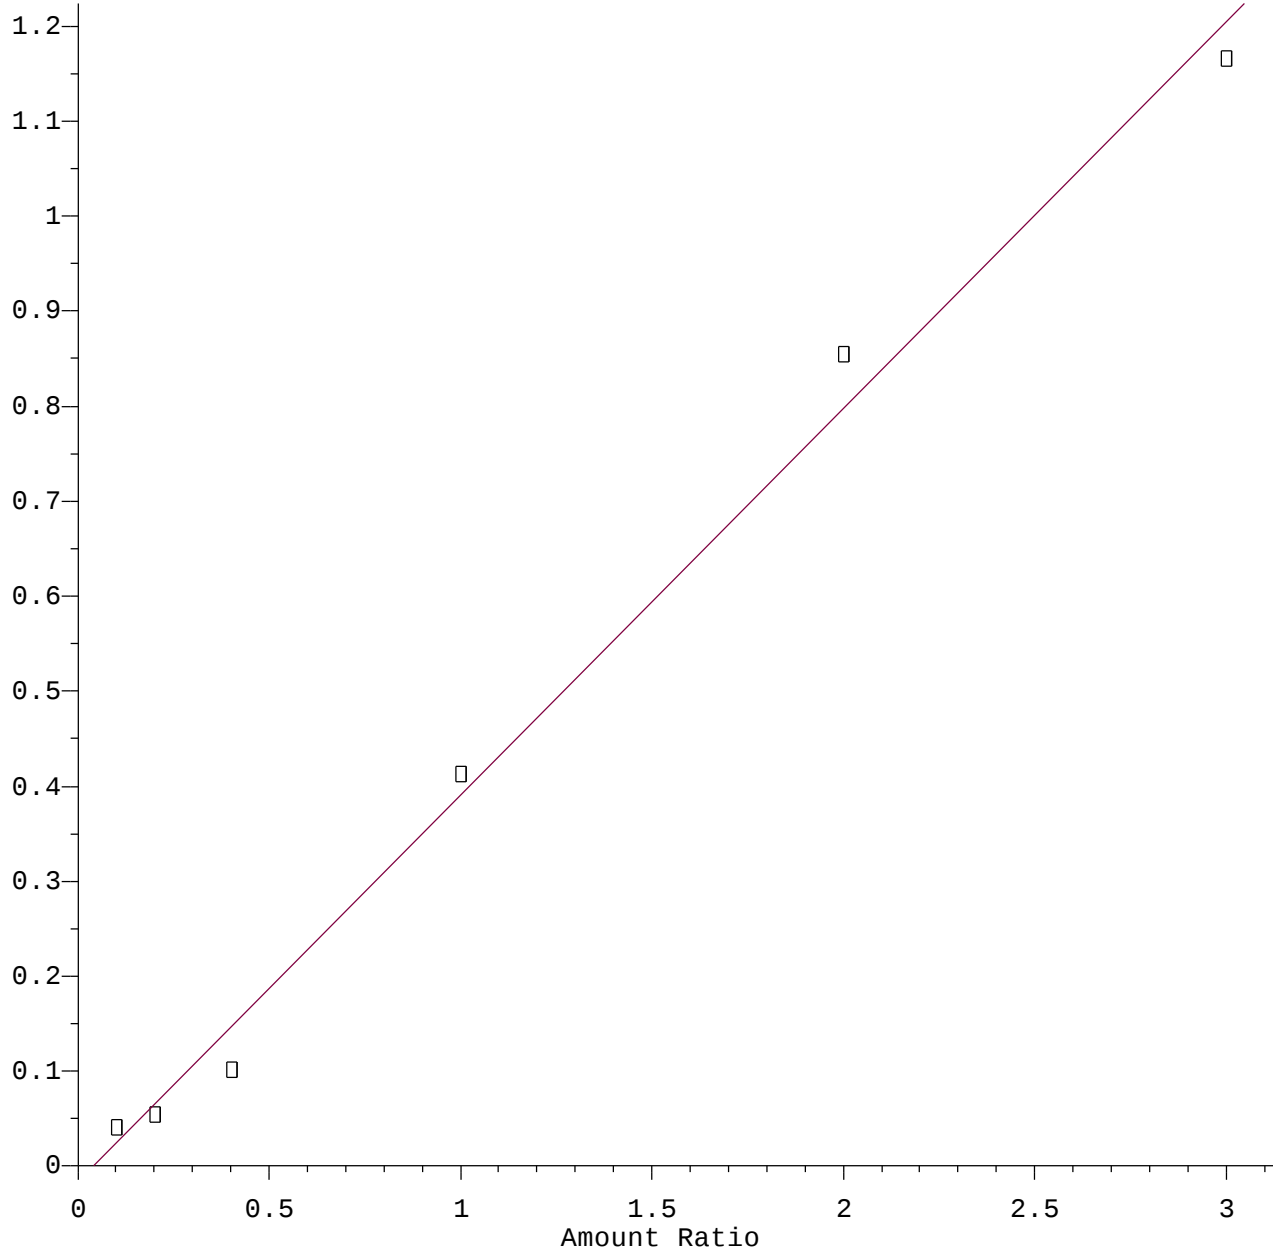

Resp Ratio = $4.07 \times 10^{-1} \times \text{Amt} - 1.64 \times 10^{-2}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y112719S.M
Calibration Table Last Updated: Wed Nov 27 12:40:47 2019