


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY112719\
 Data File : VY000807.D
 Acq On : 27 Nov 2019 09:35
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y112719S.M
 Title : SW846 8260
 Last Update : Wed Nov 27 12:40:47 2019

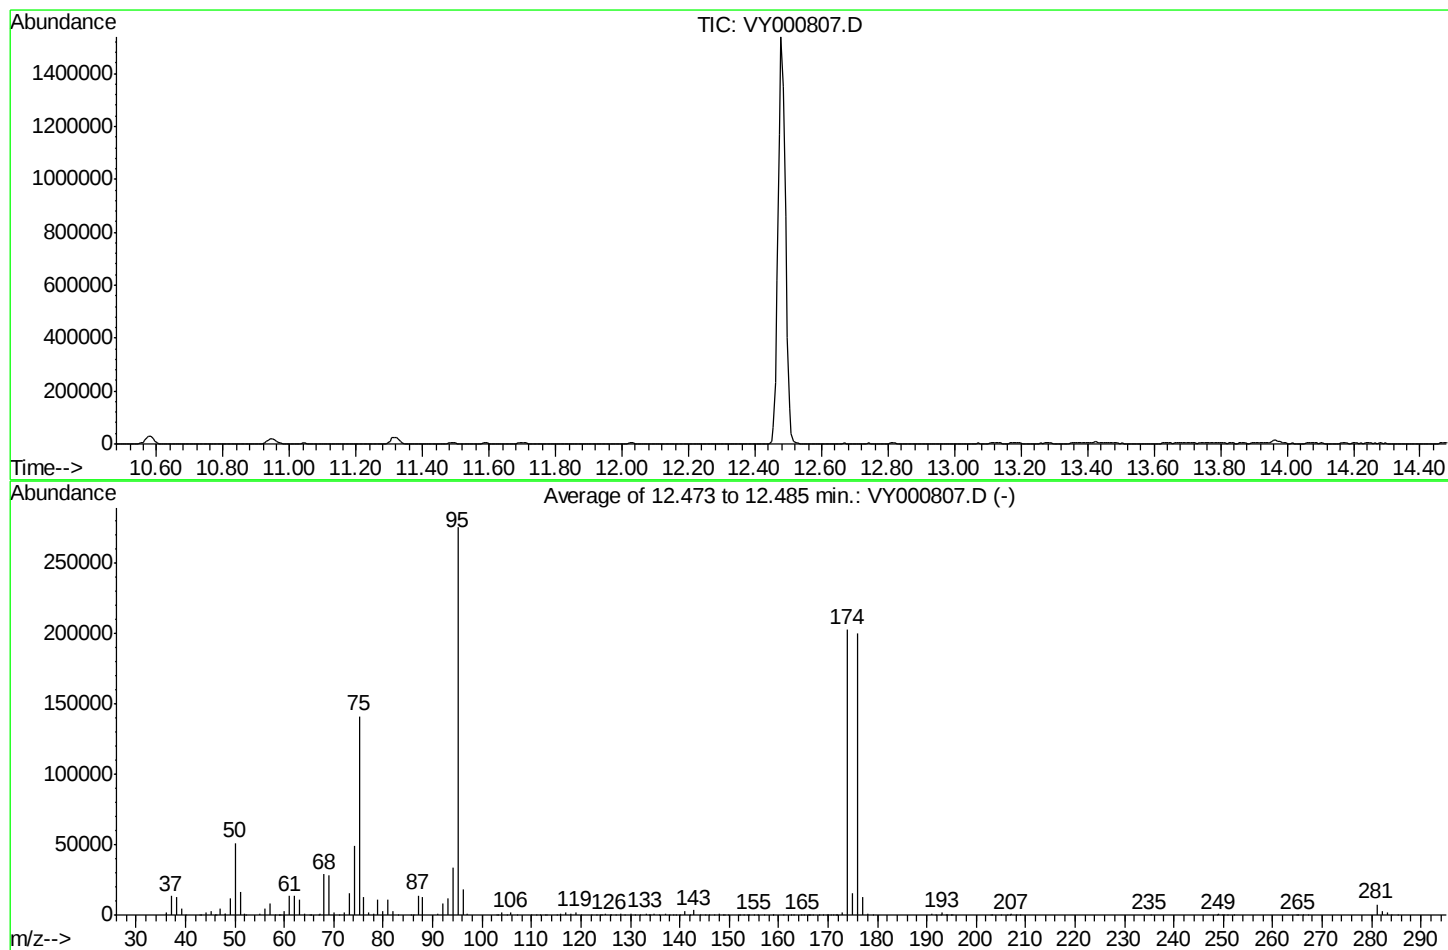

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	51290	PASS
75	95	30	60	51.2	140906	PASS
95	95	100	100	100.0	275264	PASS
96	95	5	9	6.5	17819	PASS
173	174	0.00	2	0.8	1628	PASS
174	95	50	100	73.5	202389	PASS
175	174	5	9	7.6	15336	PASS
176	174	95	101	98.7	199808	PASS
177	176	5	9	6.4	12792	PASS