
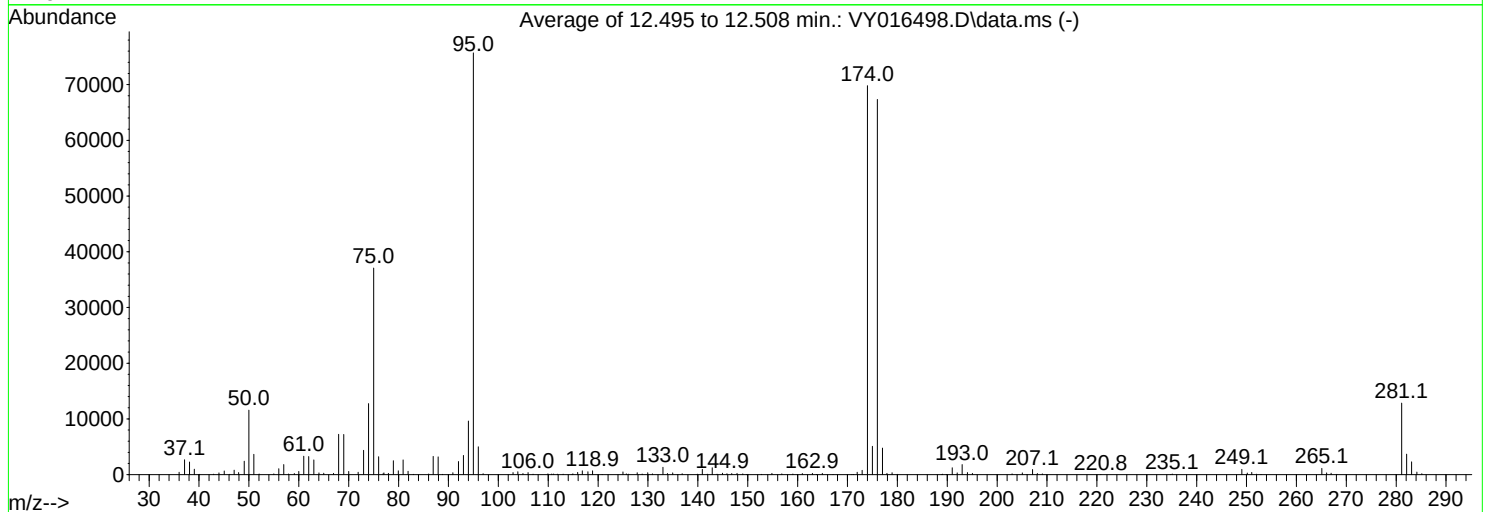


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112723\
Data File : VY016498.D
Acq On : 27 Nov 2023 09:10
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110823S.M
Title : SW846 8260
Last Update : Thu Nov 09 00:45:52 2023

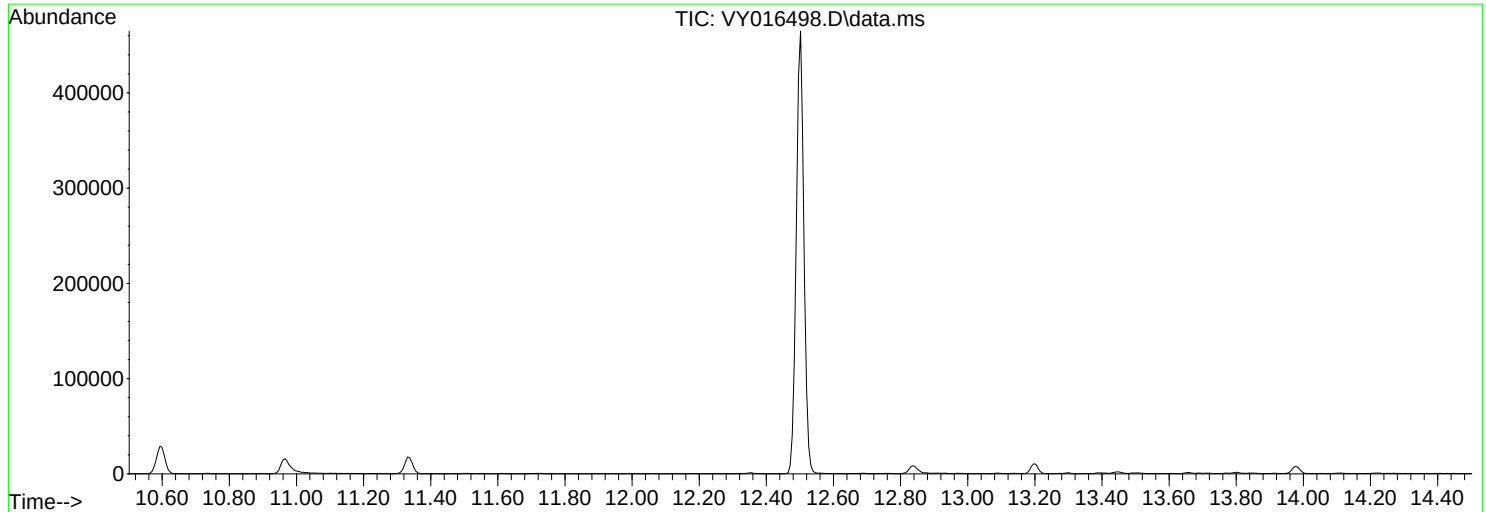

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.3	11580	PASS
75	95	30	60	49.0	37072	PASS
95	95	100	100	100.0	75699	PASS
96	95	5	9	6.6	5005	PASS
173	174	0.00	2	1.1	772	PASS
174	95	50	100	92.2	69803	PASS
175	174	5	9	7.3	5084	PASS
176	174	95	101	96.5	67331	PASS
177	176	5	9	7.1	4757	PASS