
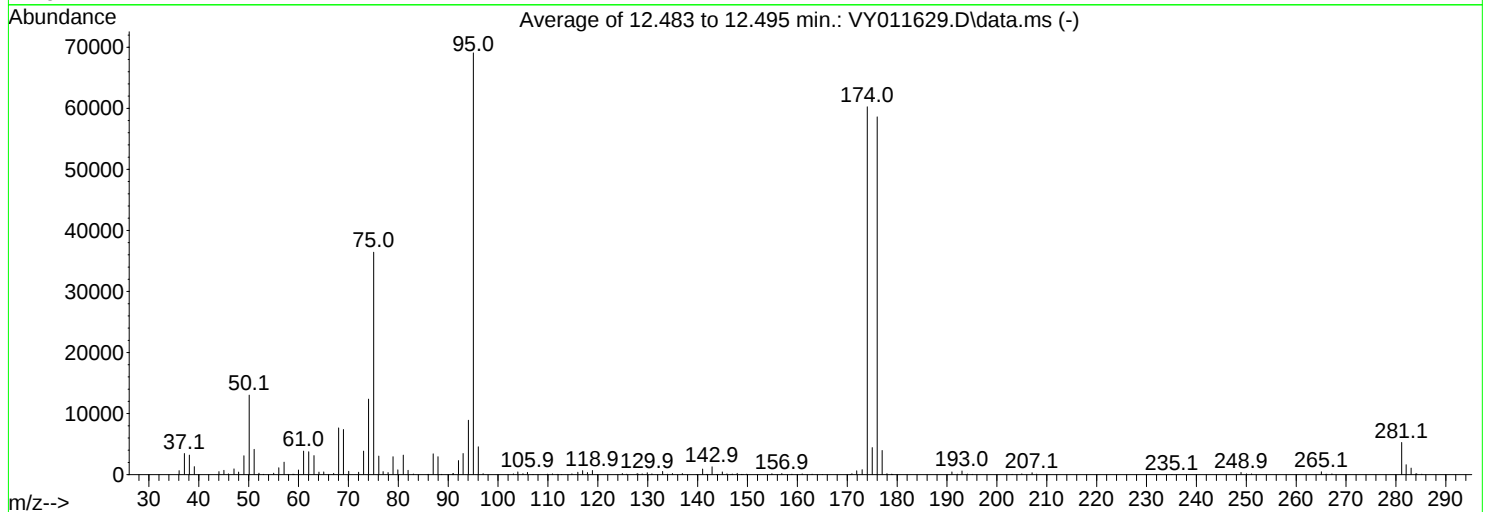


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY113022\
 Data File : VY011629.D
 Acq On : 30 Nov 2022 08:53
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111822S.M
 Title : SW846 8260
 Last Update : Sat Nov 19 22:37:14 2022

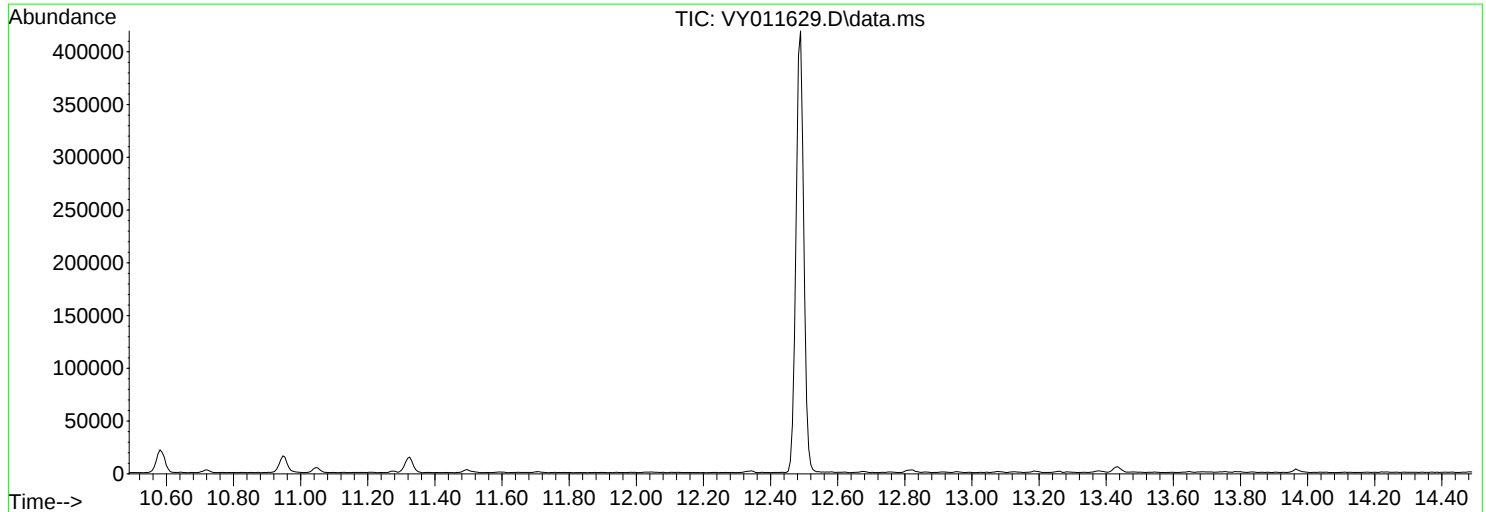

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	13035	PASS
75	95	30	60	52.7	36421	PASS
95	95	100	100	100.0	69088	PASS
96	95	5	9	6.6	4562	PASS
173	174	0.00	2	1.4	824	PASS
174	95	50	100	87.2	60256	PASS
175	174	5	9	7.4	4430	PASS
176	174	95	101	97.3	58605	PASS
177	176	5	9	6.8	3958	PASS