
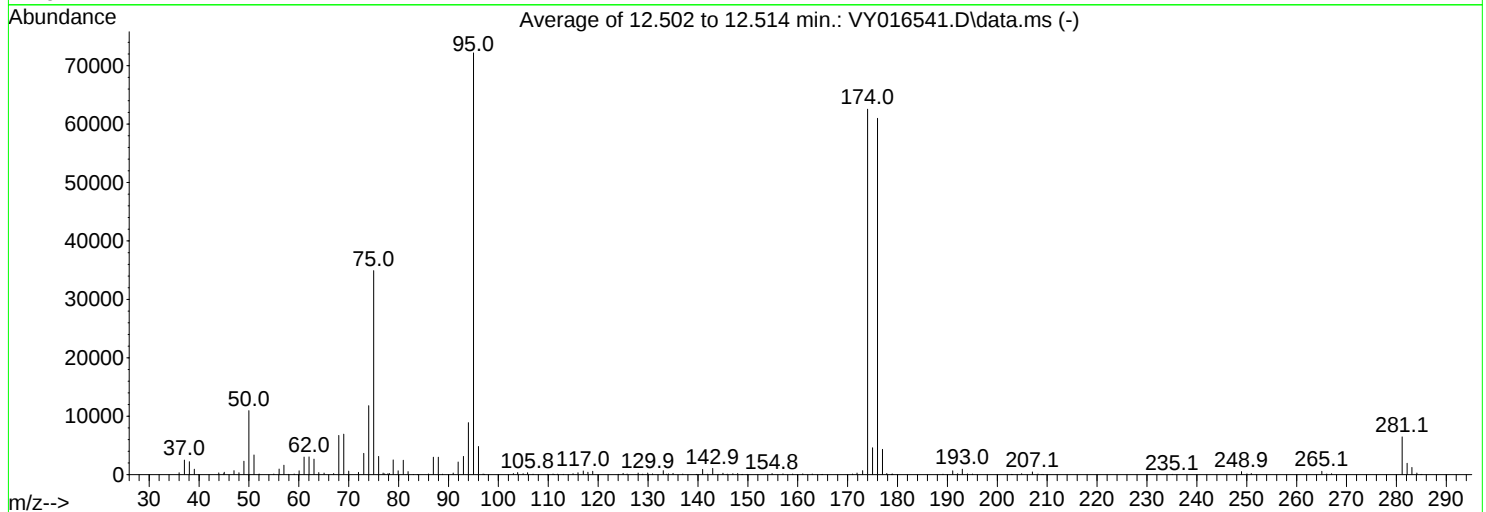


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY113023\
Data File : VY016541.D
Acq On : 30 Nov 2023 07:54
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y112923S.M
Title : SW846 8260
Last Update : Thu Nov 30 03:28:04 2023

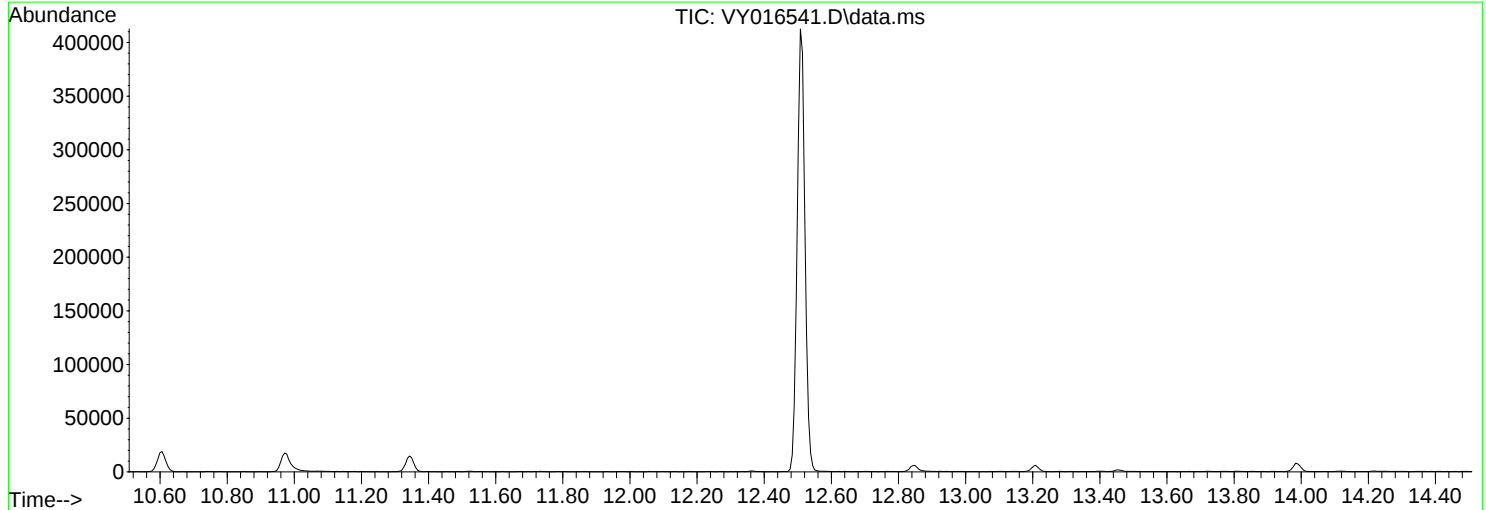

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.2	10963	PASS
75	95	30	60	48.4	34917	PASS
95	95	100	100	100.0	72200	PASS
96	95	5	9	6.7	4812	PASS
173	174	0.00	2	1.1	674	PASS
174	95	50	100	86.6	62544	PASS
175	174	5	9	7.4	4613	PASS
176	174	95	101	97.5	60992	PASS
177	176	5	9	7.1	4323	PASS