
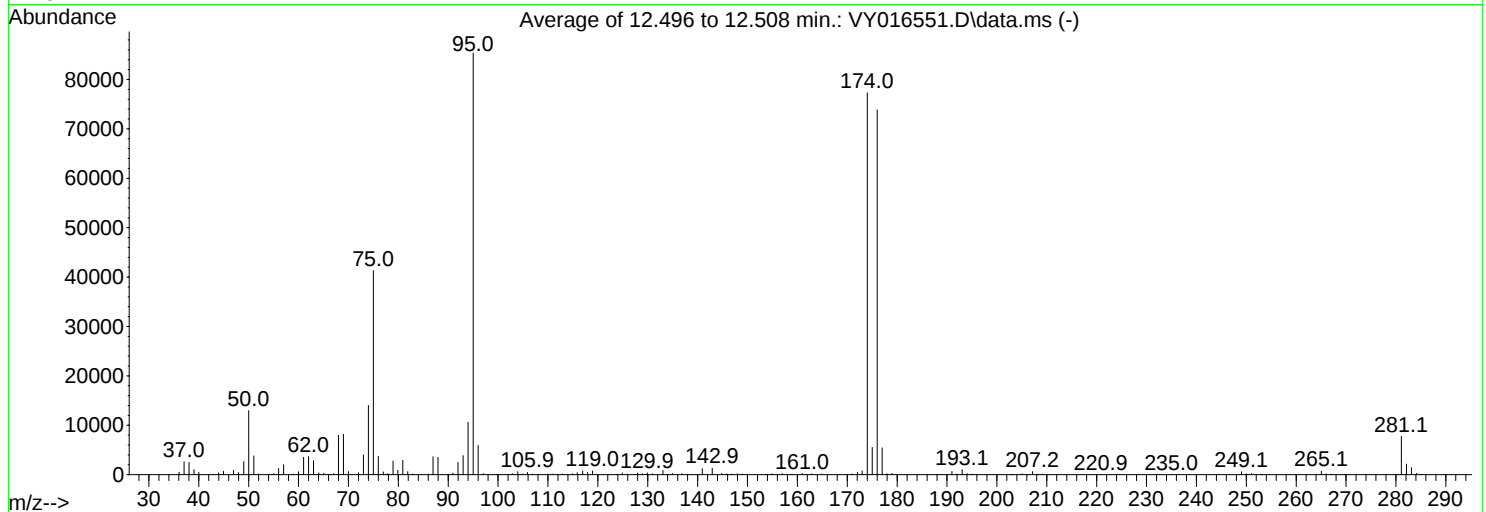


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120123\
Data File : VY016551.D
Acq On : 01 Dec 2023 08:55
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y112923S.M
Title : SW846 8260
Last Update : Thu Nov 30 03:28:04 2023

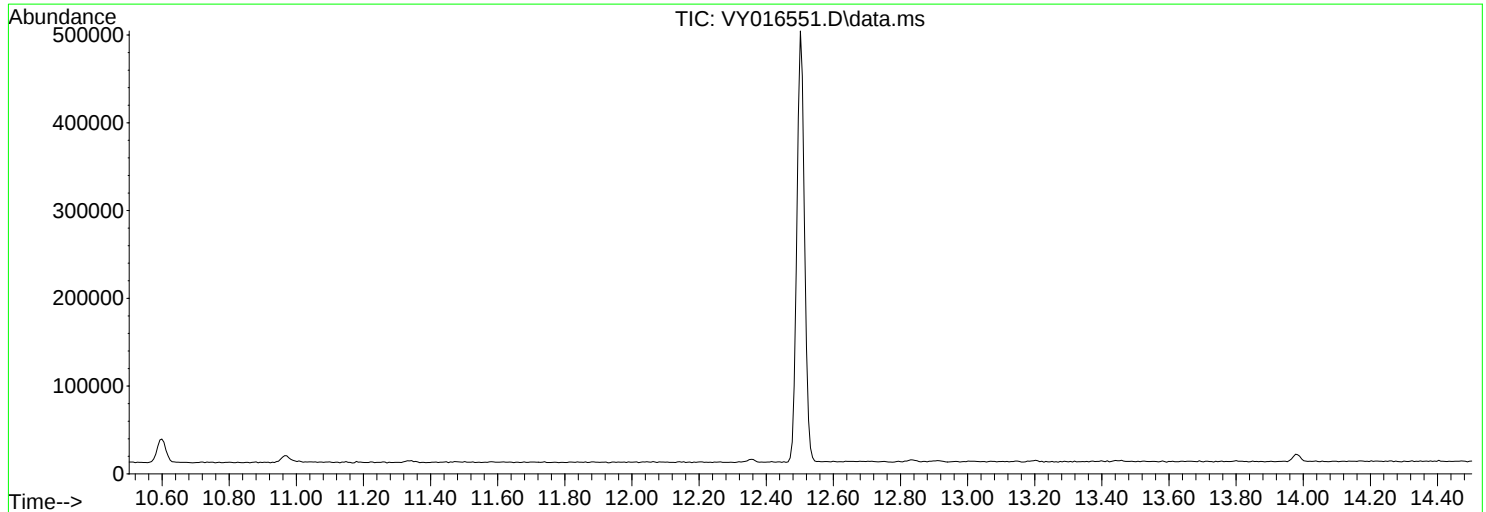

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	12948	PASS
75	95	30	60	48.4	41291	PASS
95	95	100	100	100.0	85387	PASS
96	95	5	9	6.9	5931	PASS
173	174	0.00	2	1.0	759	PASS
174	95	50	100	90.5	77301	PASS
175	174	5	9	7.1	5518	PASS
176	174	95	101	95.5	73859	PASS
177	176	5	9	7.3	5414	PASS