

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120222\
 Data File : VY011680.D
 Acq On : 02 Dec 2022 14:01
 Operator : KP/MD
 Sample : N5863-01
 Misc : 5.03g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SAND-PILE-1

Quant Time: Dec 02 23:52:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111822S.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 19 22:37:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	197752	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	357034	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	343610	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	152354	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	127416	63.455	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	126.920%
35) Dibromofluoromethane	7.716	113	112990	51.409	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.820%
50) Toluene-d8	10.179	98	433170	54.235	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	108.480%
62) 4-Bromofluorobenzene	12.483	95	142222	48.162	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	96.320%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120222\
Data File : VY011680.D
Acq On : 02 Dec 2022 14:01
Operator : KP/MD
Sample : N5863-01
Misc : 5.03g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SAND-PILE-1

Quant Time: Dec 02 23:52:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111822S.M
Quant Title : SW846 8260
QLast Update : Sat Nov 19 22:37:14 2022
Response via : Initial Calibration




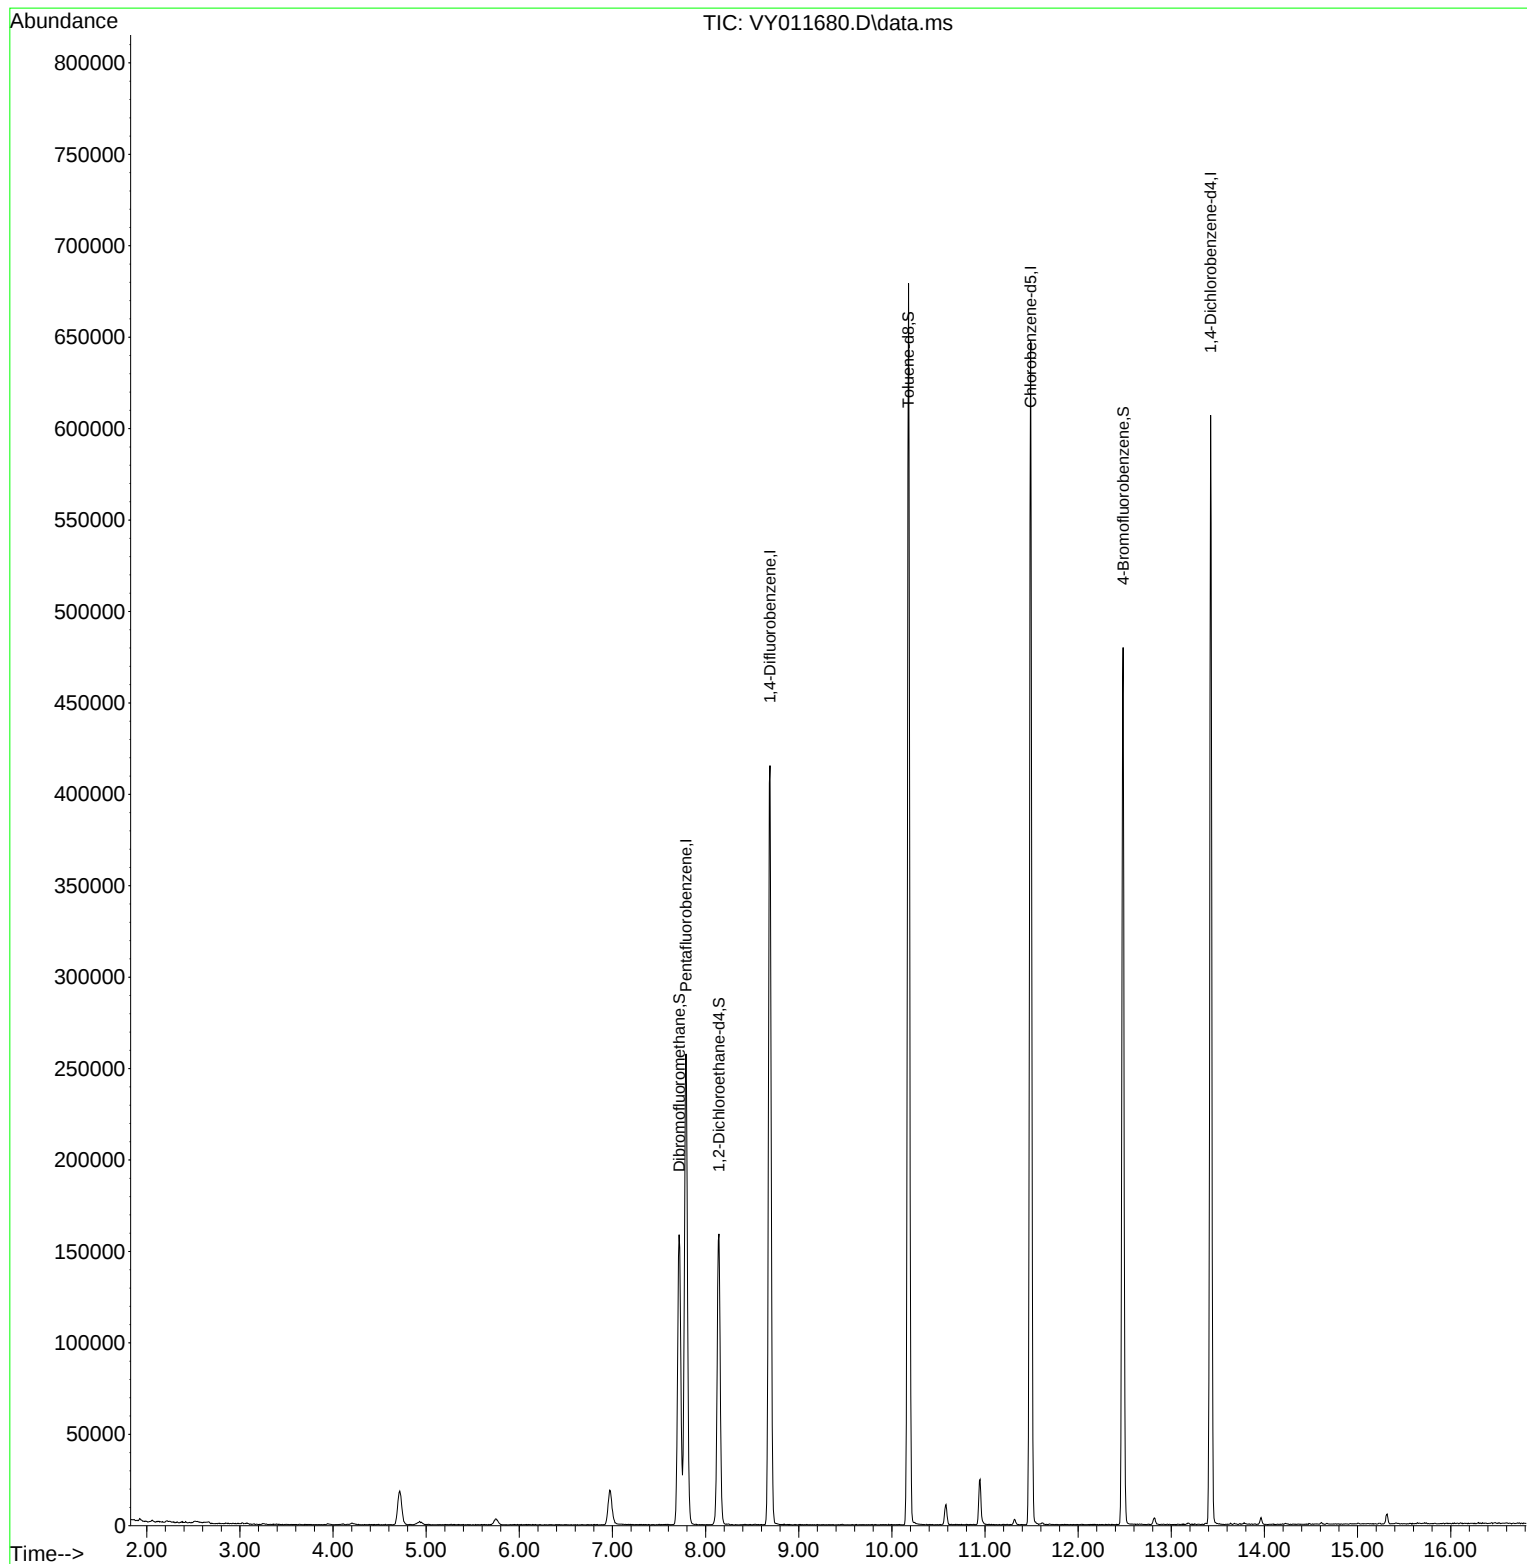




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY011680.D
Acq: 02 Dec 2022 14:01




Instrument :
MSVOA_Y
ClientSampleId :
SAND-PILE-1

Tgt Ion:168 Resp: 197752
Ion Ratio Lower Upper
168 100
99 58.4 46.9 70.3

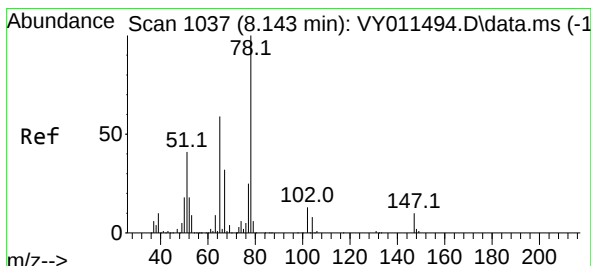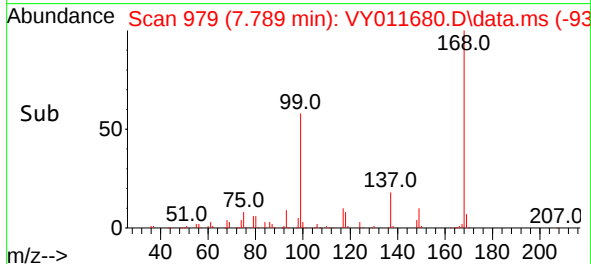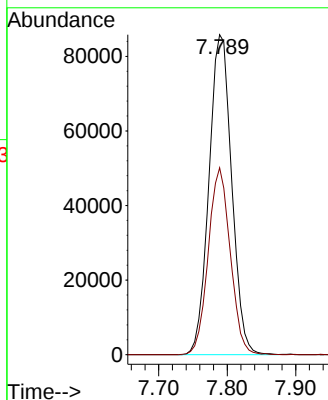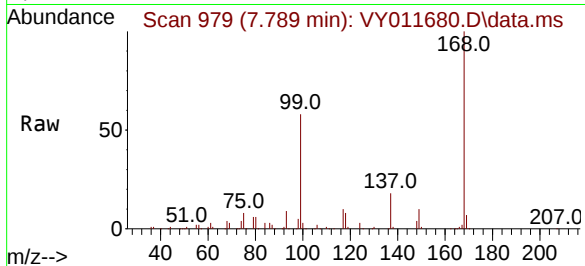

#33
1,2-Dichloroethane-d4
Concen: 63.455 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VY011680.D
Acq: 02 Dec 2022 14:01

Tgt Ion: 65 Resp: 127416
Ion Ratio Lower Upper
65 100
67 51.9 0.0 99.4

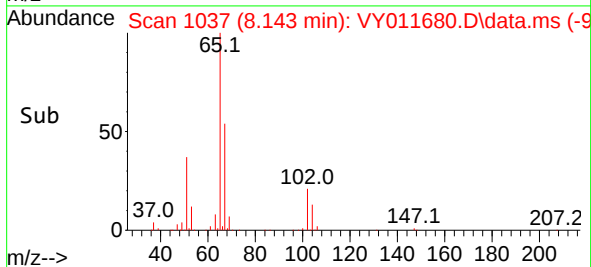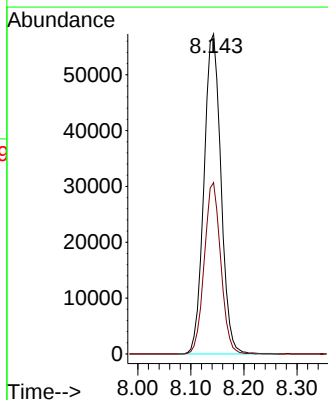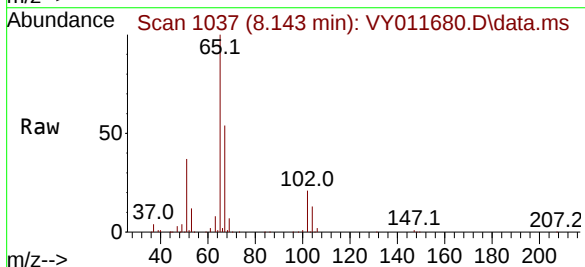



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY011680.D

Acq: 02 Dec 2022 14:01

Instrument :

MSVOA_Y

ClientSampleId :

SAND-PILE-1





Tgt Ion:114 Resp: 357034

Ion Ratio Lower Upper

114 100

63 20.4 0.0 43.2

88 15.4 0.0 31.8

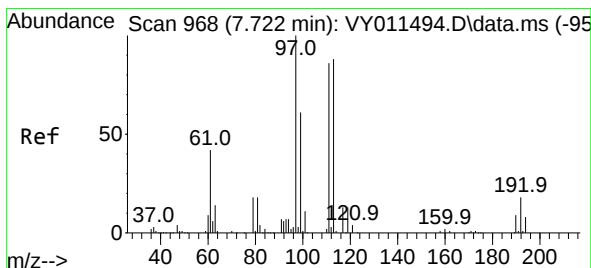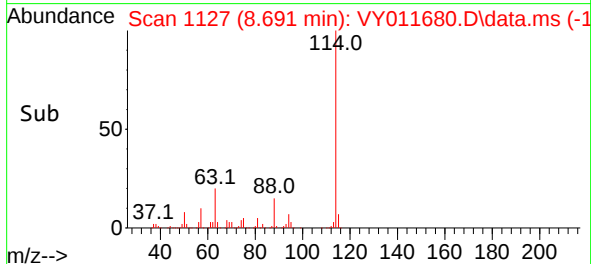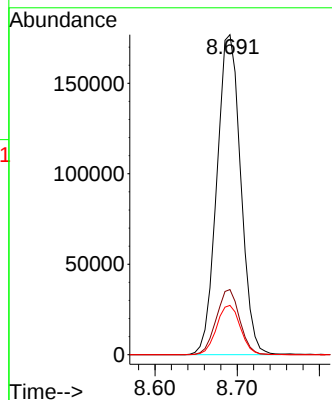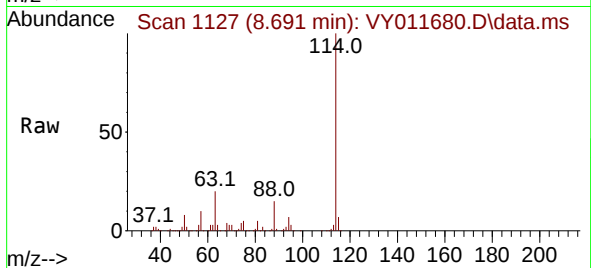

#35

Dibromofluoromethane

Concen: 51.409 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.006 min

Lab File: VY011680.D

Acq: 02 Dec 2022 14:01




Tgt Ion:113 Resp: 112990


Ion Ratio Lower Upper

113 100

111 102.9 82.6 124.0

192 19.9 17.6 26.4

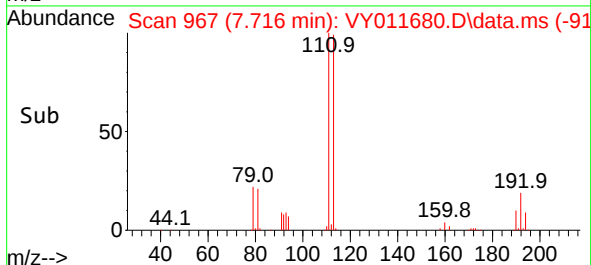
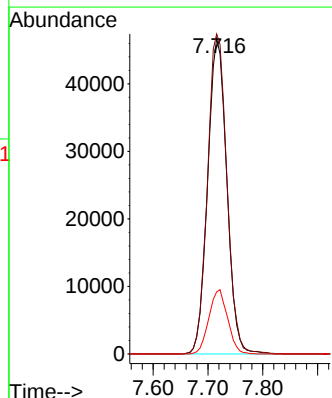
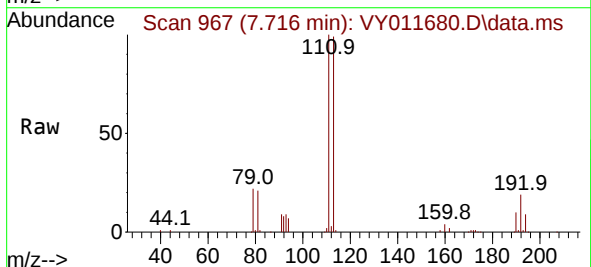


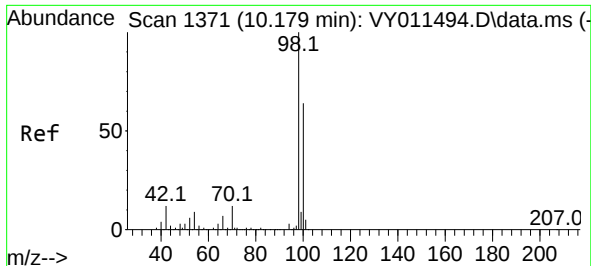

#50
Toluene-d8
Concen: 54.235 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY011680.D
Acq: 02 Dec 2022 14:01




Instrument :
MSVOA_Y
ClientSampleId :
SAND-PILE-1


Tgt Ion: 98 Resp: 433170
Ion Ratio Lower Upper
98 100
100 63.8 50.2 75.2

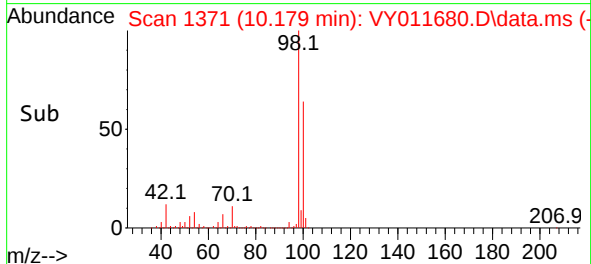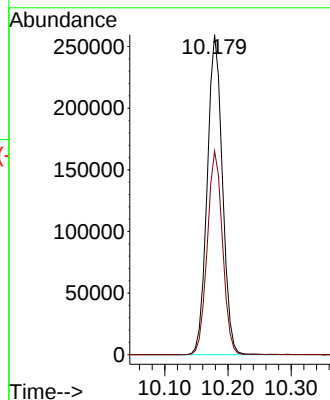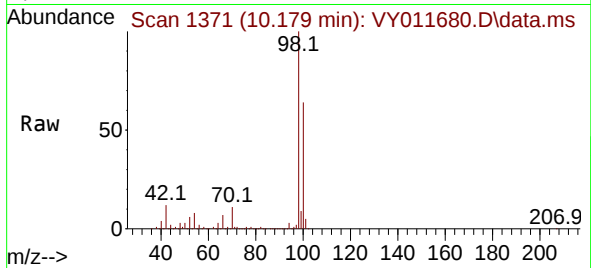

#62
4-Bromofluorobenzene
Concen: 48.162 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY011680.D
Acq: 02 Dec 2022 14:01

Tgt Ion: 95 Resp: 142222
Ion Ratio Lower Upper
95 100
174 84.9 0.0 177.0
176 81.6 0.0 175.8


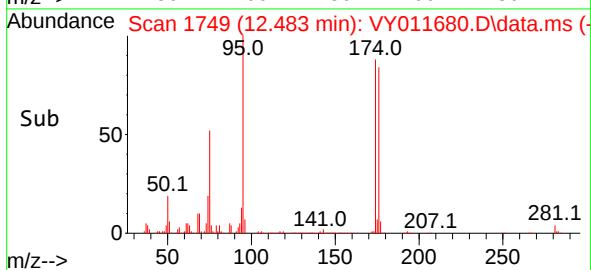
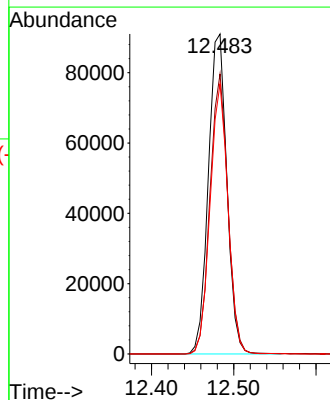
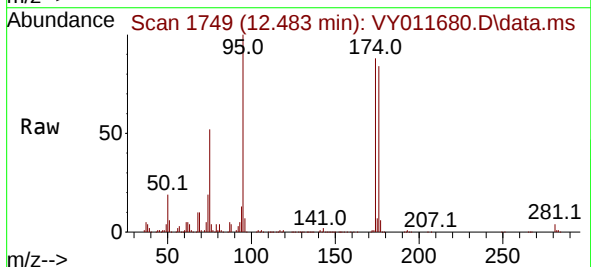


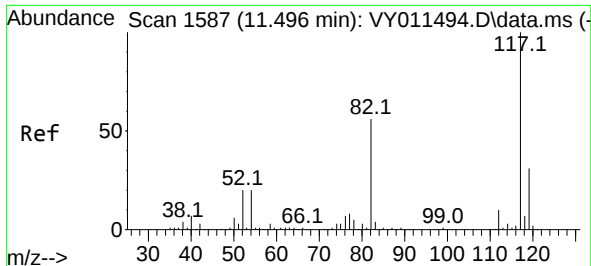

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 117
Delta R.T. -0.006 min
Lab File: VY011680.D
Acq: 02 Dec 2022 14:01

Instrument :
MSVOA_Y
ClientSampleId :
SAND-PILE-1

Tgt Ion:117 Resp: 343610
Ion Ratio Lower Upper
117 100
82 56.5 43.0 64.4
119 33.1 25.4 38.0

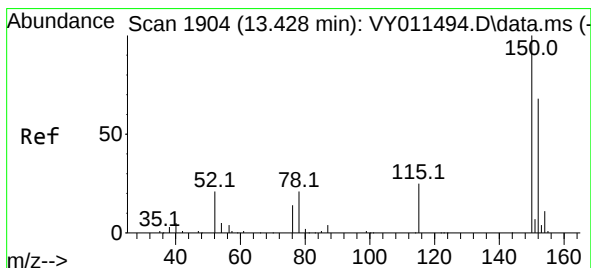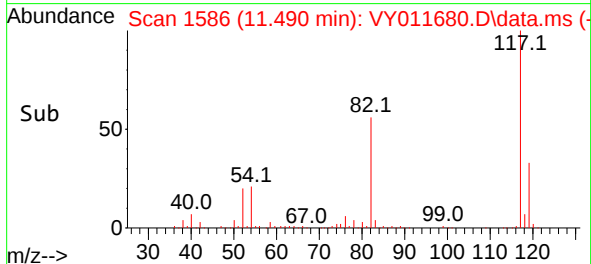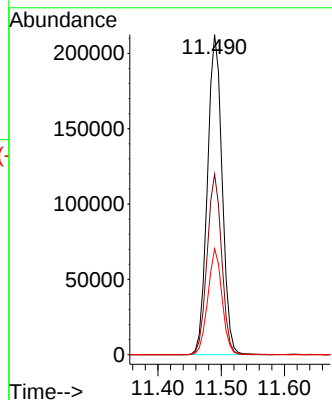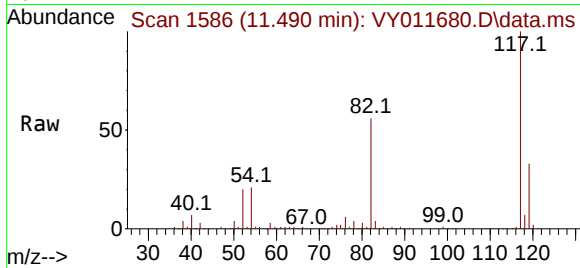

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.006 min
Lab File: VY011680.D
Acq: 02 Dec 2022 14:01

Tgt Ion:152 Resp: 152354
Ion Ratio Lower Upper
152 100
115 58.0 28.2 84.7
150 155.7 0.0 347.6

