
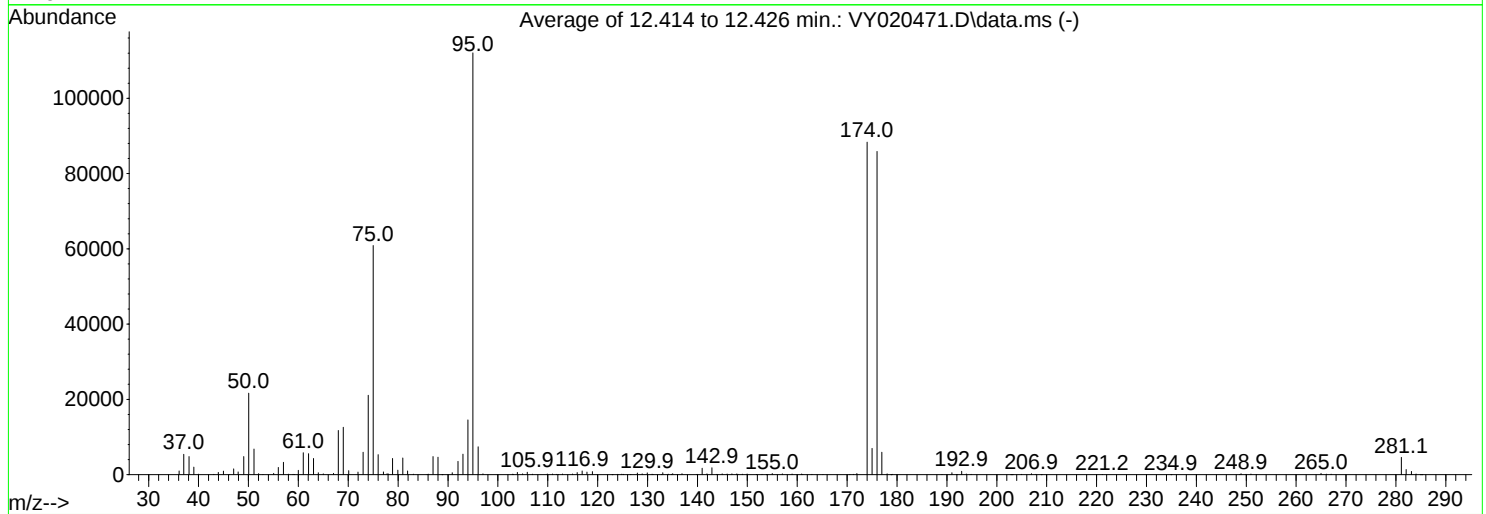


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120224\
Data File : VY020471.D
Acq On : 02 Dec 2024 08:23
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120224S.M
Title : SW846 8260
Last Update : Tue Dec 03 01:39:23 2024

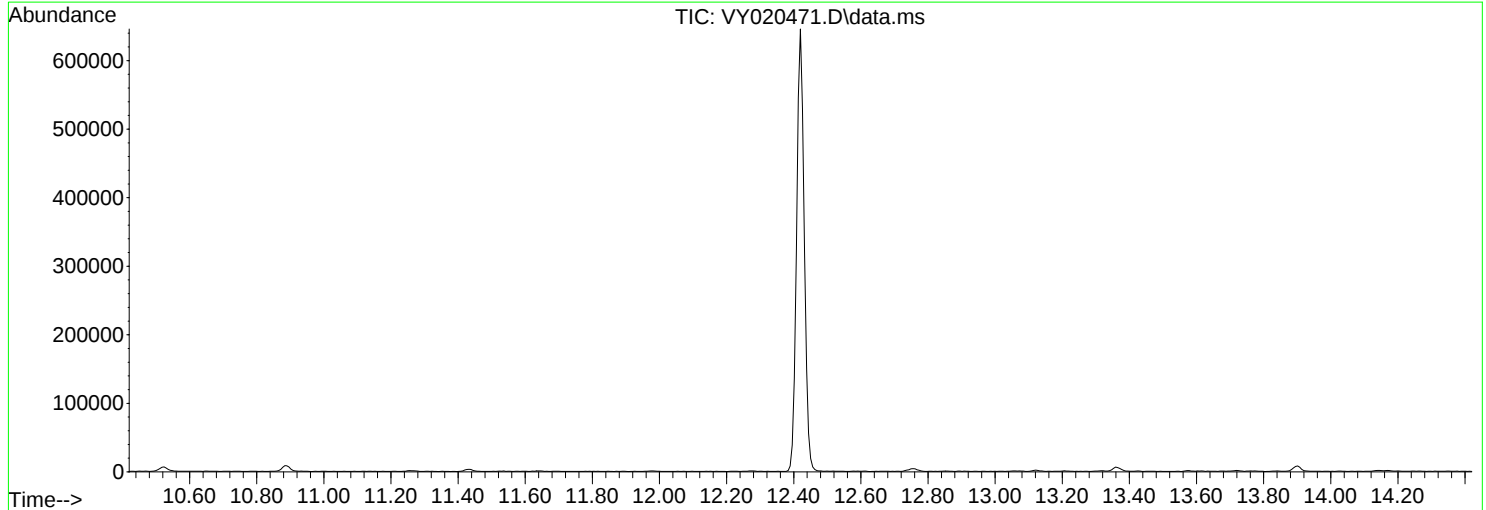

AutoFind: Scans 1754, 1755, 1756; Background Corrected with Scan 1746

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	21643	PASS
75	95	30	60	54.3	60867	PASS
95	95	100	100	100.0	112075	PASS
96	95	5	9	6.6	7403	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.8	88365	PASS
175	174	5	9	7.9	6989	PASS
176	174	95	101	97.2	85864	PASS
177	176	5	9	6.9	5960	PASS