


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv120319\
Data File : VY000831.D
Acq On : 03 Dec 2019 09:45
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y112719S.M
Title : SW846 8260
Last Update : Wed Nov 27 12:40:47 2019

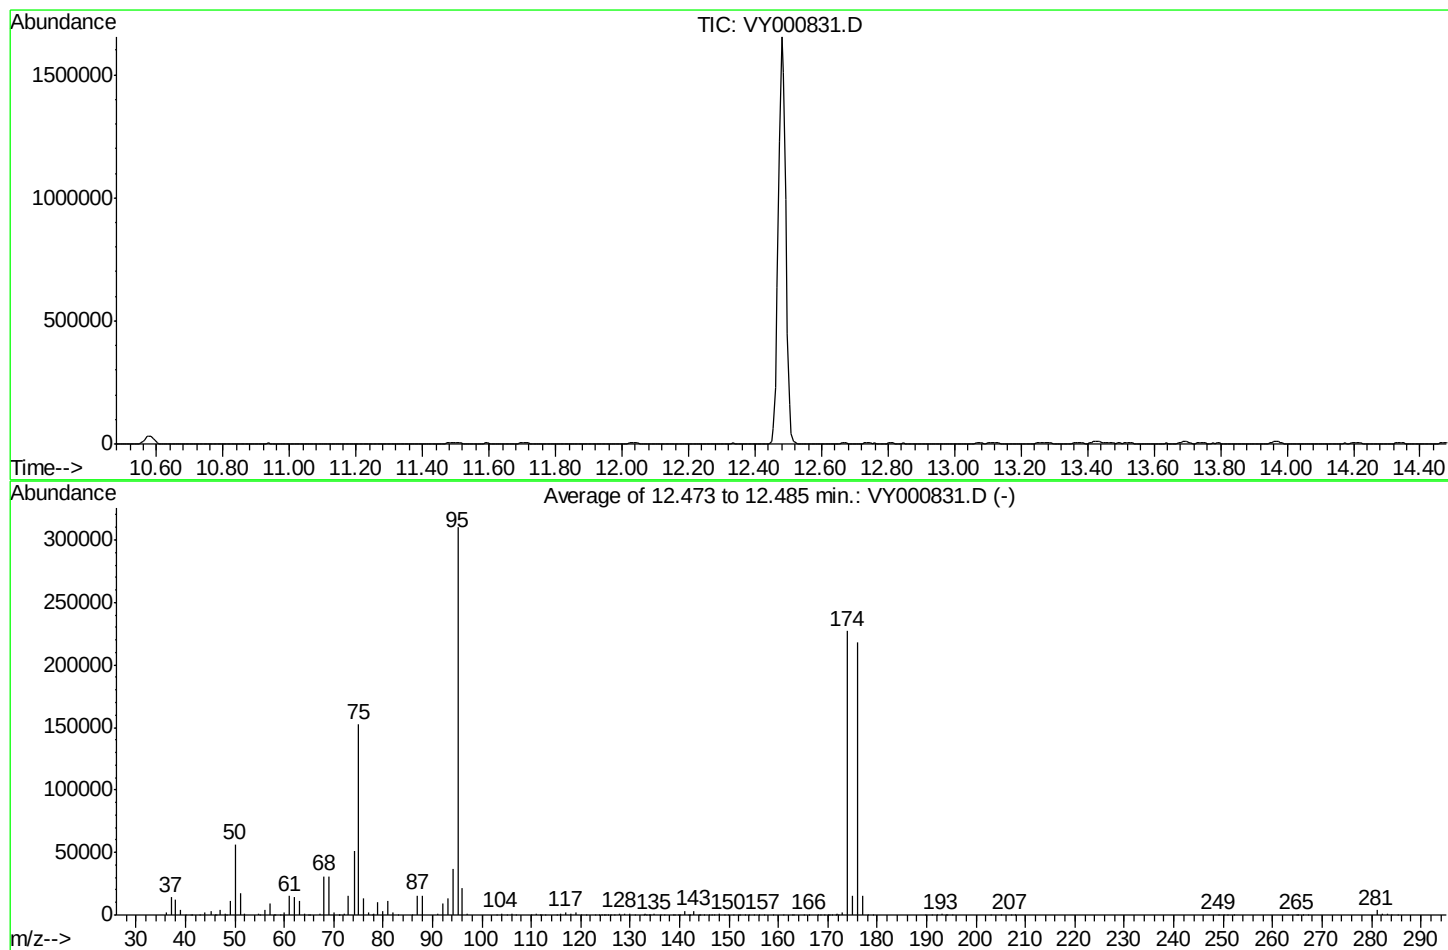

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	56285	PASS
75	95	30	60	49.2	152512	PASS
95	95	100	100	100.0	310058	PASS
96	95	5	9	6.9	21354	PASS
173	174	0.00	2	0.8	1759	PASS
174	95	50	100	73.3	227178	PASS
175	174	5	9	6.9	15566	PASS
176	174	95	101	96.0	218176	PASS
177	176	5	9	6.8	14936	PASS