


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv120419\  
 Data File : VY000851.D  
 Acq On : 04 Dec 2019 09:50  
 Operator : SY/MD  
 Sample : BFB  
 Misc : 5.00G/5ML/MSVOA Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_Y\METHODS\82Y112719S.M  
 Title : SW846 8260  
 Last Update : Wed Nov 27 12:40:47 2019

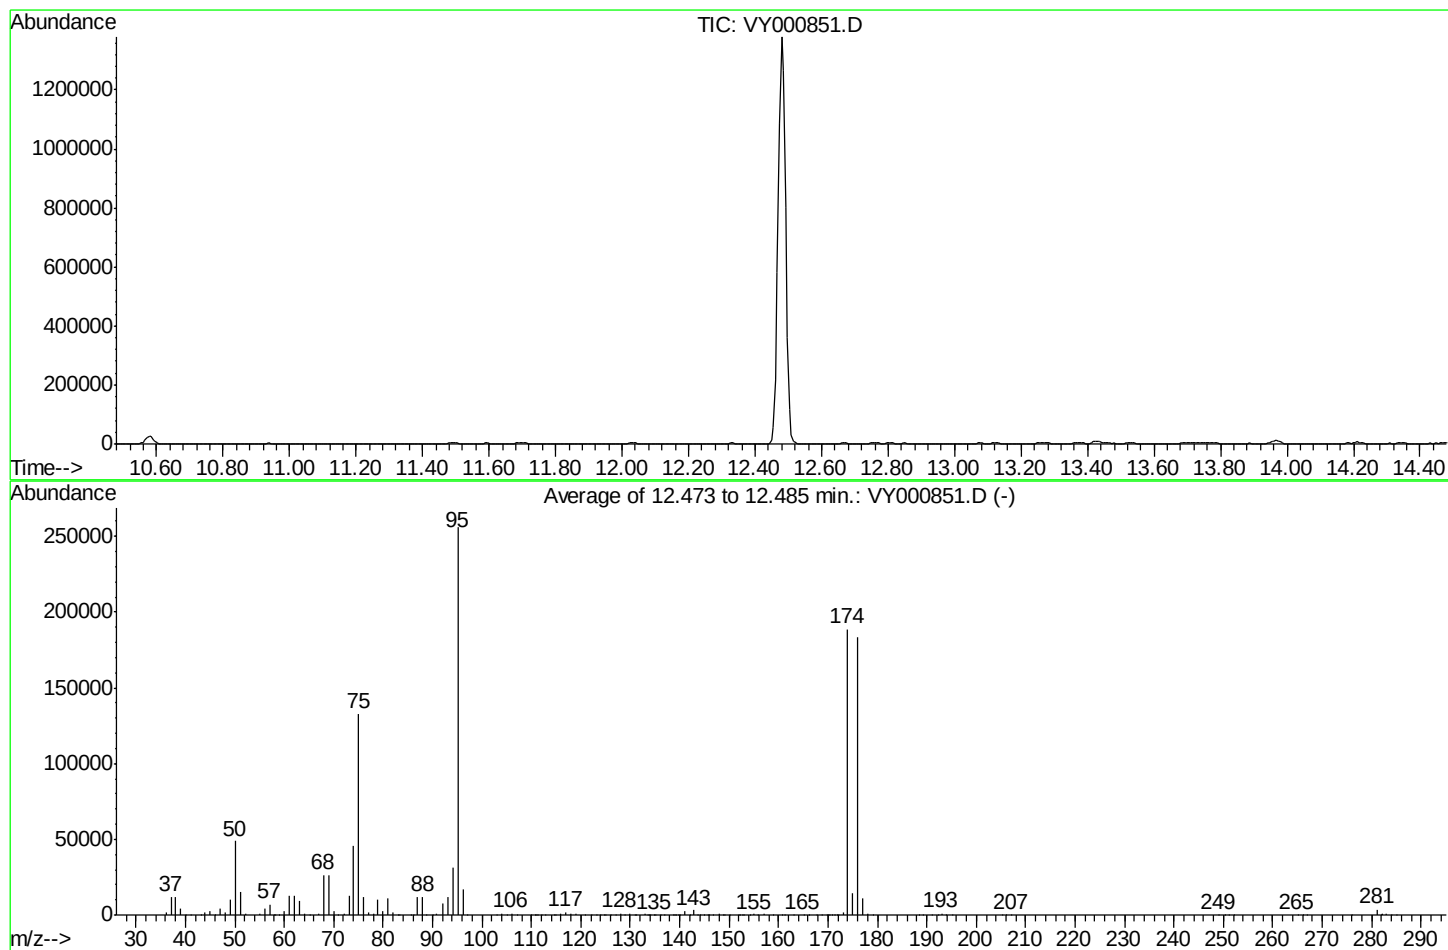

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.1      | 48874   | PASS             |
| 75          | 95           | 30           | 60           | 52.0      | 133178  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 256042  | PASS             |
| 96          | 95           | 5            | 9            | 6.7       | 17130   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.7       | 1343    | PASS             |
| 174         | 95           | 50           | 100          | 73.7      | 188757  | PASS             |
| 175         | 174          | 5            | 9            | 7.5       | 14155   | PASS             |
| 176         | 174          | 95           | 101          | 97.4      | 183829  | PASS             |
| 177         | 176          | 5            | 9            | 6.0       | 11064   | PASS             |