

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120421\
 Data File : VY006951.D
 Acq On : 04 Dec 2021 18:43
 Operator : SY/MD
 Sample : M4884-21
 Misc : 4.89g/10.0mL/MSVOA_Y/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 EW9K5

Quant Time: Dec 05 06:09:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\SFAMYL120321SMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 04 02:26:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.691	114	125896	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.490	117	100752	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.422	152	27341	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.247	65	59557	36.731	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	146.920%
7) Chloroethane-d5	2.772	69	42656	33.536	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	134.160%
11) 1,1-Dichloroethene-d2	3.851	63	65155	19.329	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	77.320%
21) 2-Butanone-d5	6.887	46	38734	61.850	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	123.700%
24) Chloroform-d	7.478	84	84485	26.928	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	107.720%
26) 1,2-Dichloroethane-d4	8.143	65	52200	27.718	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	110.880%
32) Benzene-d6	8.112	84	162581	30.378	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	121.520%
36) 1,2-Dichloropropane-d6	9.124	67	55420	32.958	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	131.840%#
41) Toluene-d8	10.179	98	143436	28.615	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	114.480%
43) trans-1,3-Dichloroprop...	10.435	79	23035	28.321	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	113.280%
47) 2-Hexanone-d5	10.788	63	24872	63.908	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	127.820%
56) 1,1,2,2-Tetrachloroeth...	12.563	84	41532	29.646	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	118.600%
66) 1,2-Dichlorobenzene-d4	13.721	152	26108	29.282	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	117.120%
Target Compounds						Qvalue
13) Acetone	3.948	43	1688	2.941	ug/L	58
27) 1,2-Dichloroethane	8.240	62	2017	0.809	ug/L	97
34) Trichloroethene	8.941	95	118718	71.156	ug/L	91
46) Tetrachloroethene	10.721	164	12028	8.605	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120421\
Data File : VY006951.D
Acq On : 04 Dec 2021 18:43
Operator : SY/MD
Sample : M4884-21
Misc : 4.89g/10.0mL/MSVOA_Y/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
EW9K5

Quant Time: Dec 05 06:09:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\SFAMYL120321SMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 04 02:26:29 2021
Response via : Initial Calibration




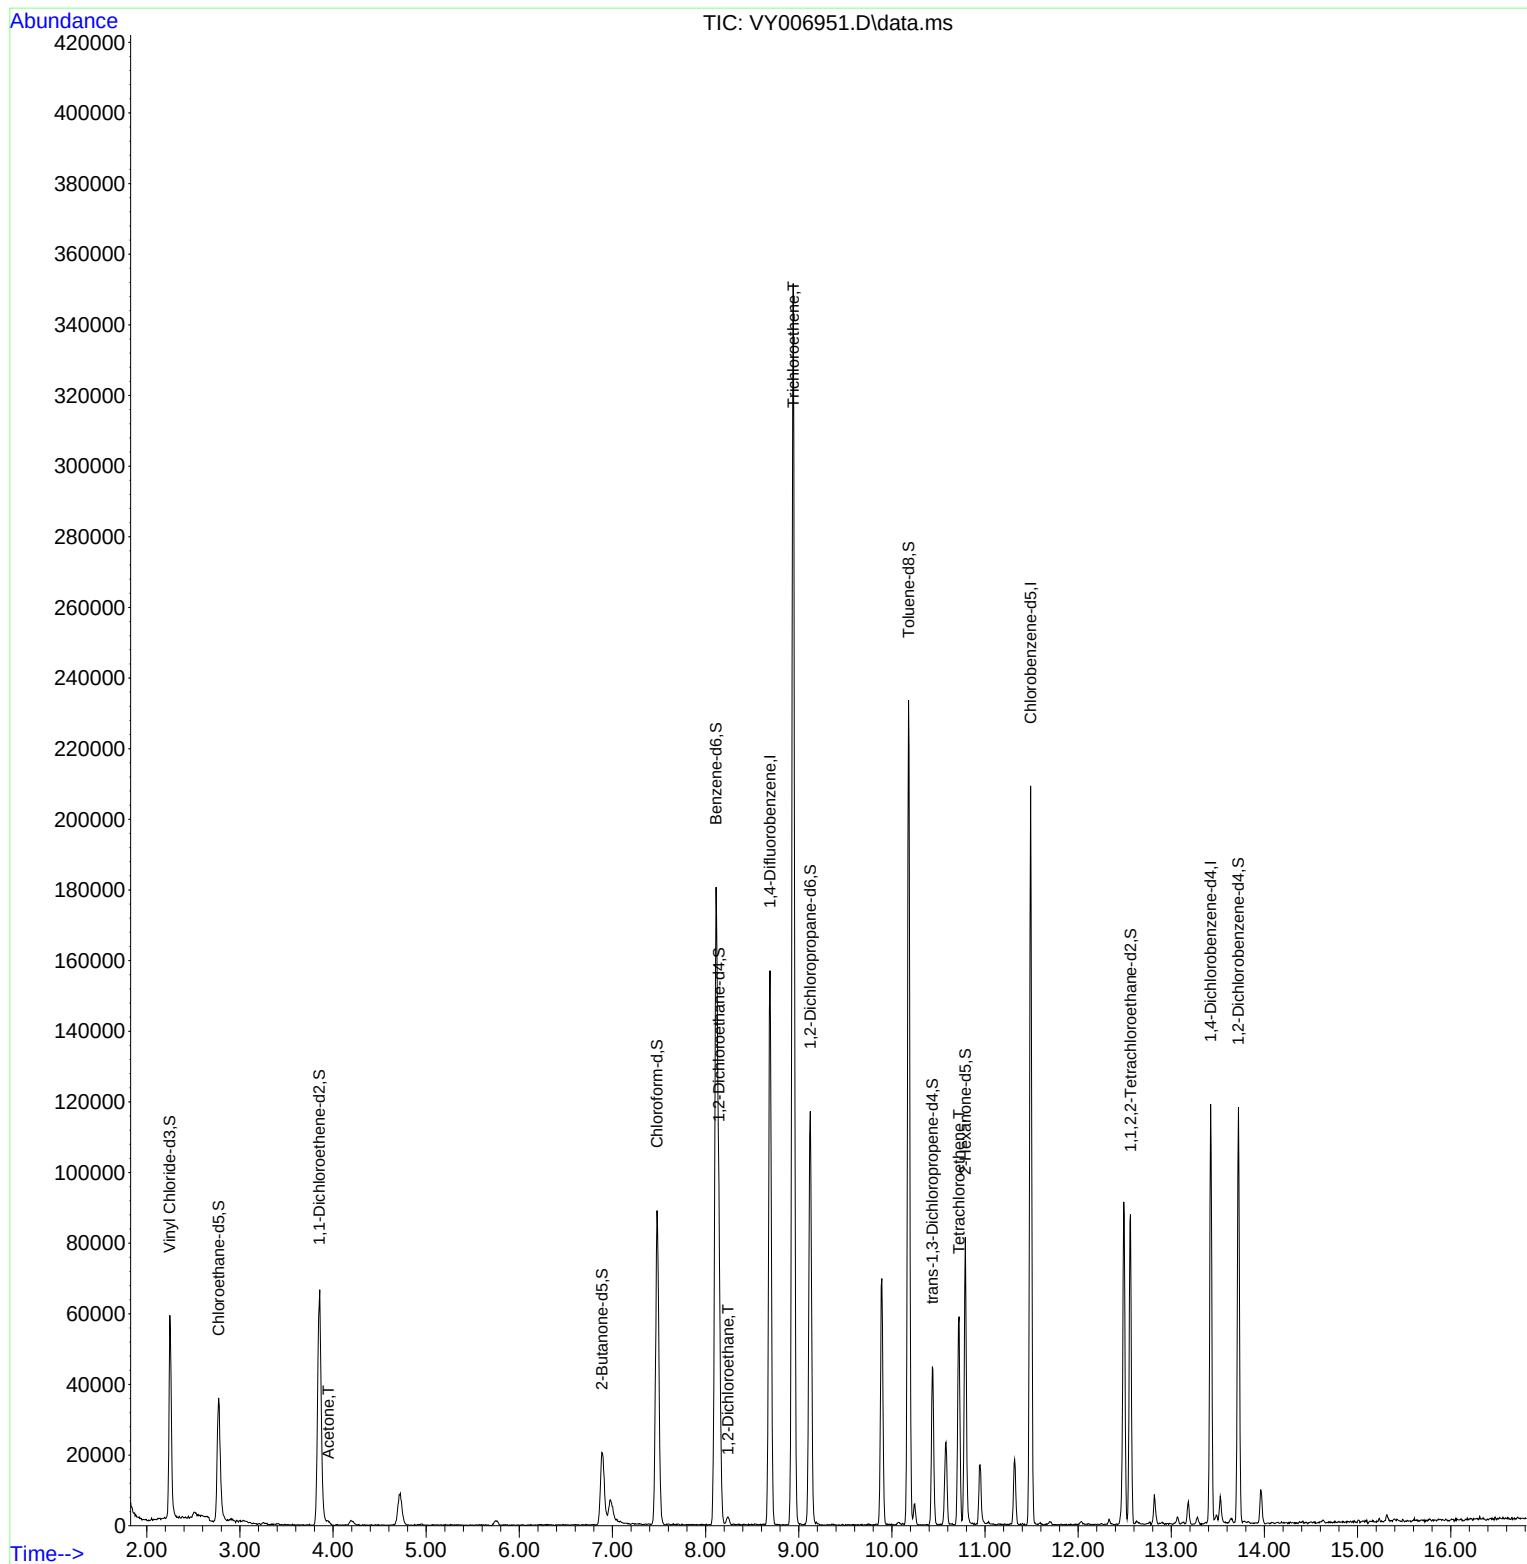


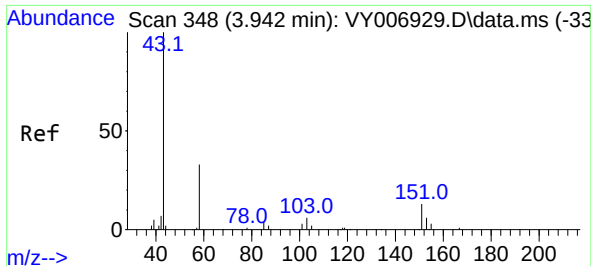

#13
Acetone
Concen: 2.941 ug/L
RT: 3.948 min Scan# 34
Delta R.T. 0.006 min
Lab File: VY006951.D
Acq: 04 Dec 2021 18:43




Instrument :
MSVOA_Y
ClientSampleId :
EW9K5


Tgt Ion: 43 Resp: 1688
Ion Ratio Lower Upper
43 100
58 7.8 0.0 60.8

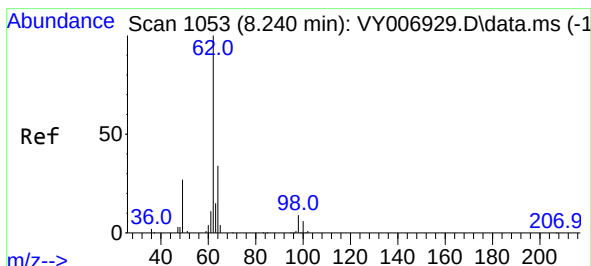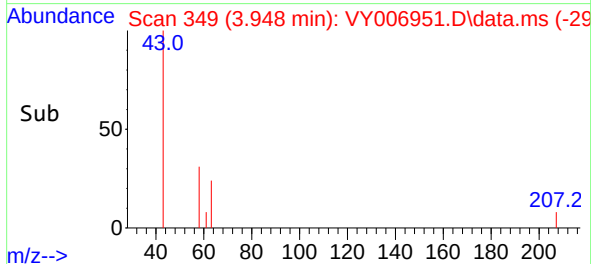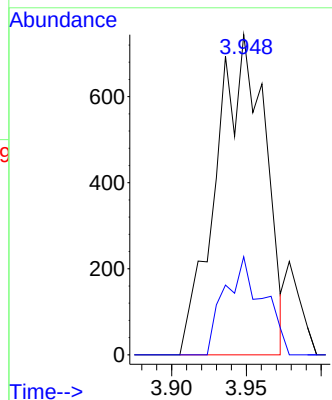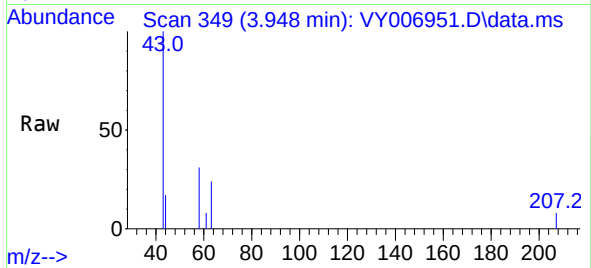

#27
1,2-Dichloroethane
Concen: 0.809 ug/L
RT: 8.240 min Scan# 1053
Delta R.T. -0.000 min
Lab File: VY006951.D
Acq: 04 Dec 2021 18:43


Tgt Ion: 62 Resp: 2017
Ion Ratio Lower Upper
62 100
98 7.4 6.9 10.3

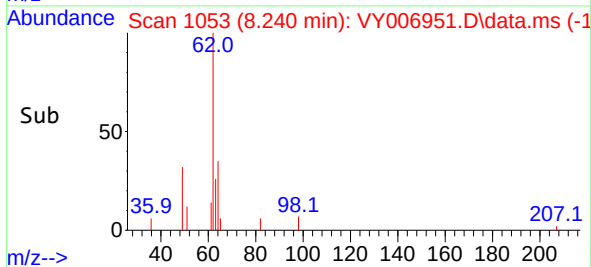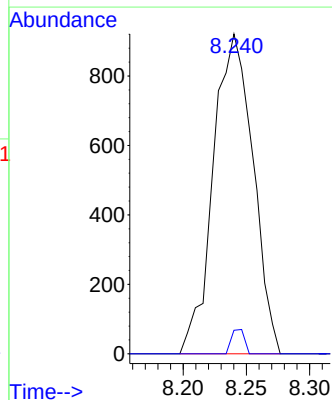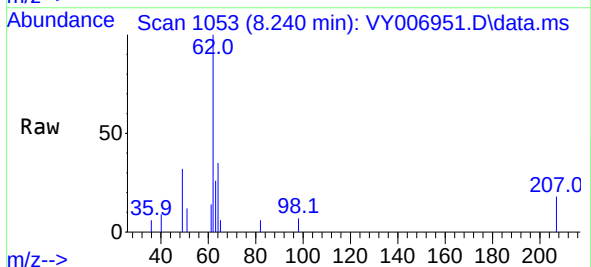



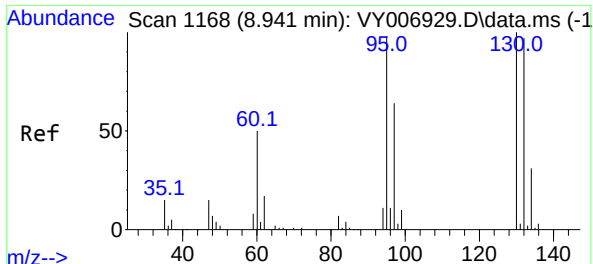


#34
Trichloroethene
Concen: 71.156 ug/L
RT: 8.941 min Scan# 1168
Delta R.T. -0.000 min
Lab File: VY006951.D
Acq: 04 Dec 2021 18:43

Instrument :
MSVOA_Y
ClientSampleId :
EW9K5

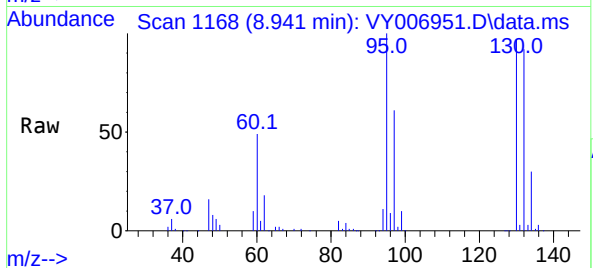

Tgt Ion: 95 Resp: 118718
Ion Ratio Lower Upper
95 100
97 60.7 47.3 87.8
132 92.3 71.3 132.5
130 97.5 74.2 137.8

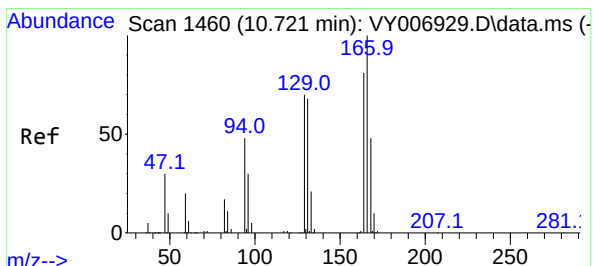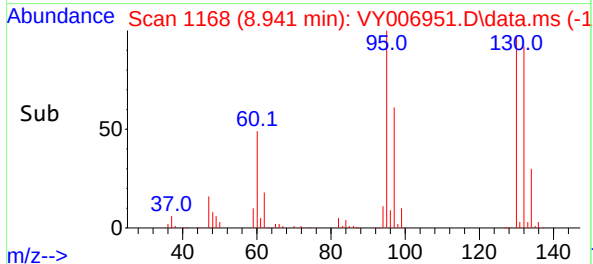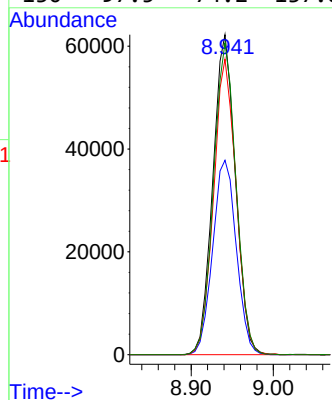

#46
Tetrachloroethene
Concen: 8.605 ug/L
RT: 10.721 min Scan# 1460
Delta R.T. -0.000 min
Lab File: VY006951.D
Acq: 04 Dec 2021 18:43

Tgt Ion: 164 Resp: 12028
Ion Ratio Lower Upper
164 100
129 98.0 62.1 115.3
131 93.0 61.0 113.2
166 122.3 90.4 168.0

