
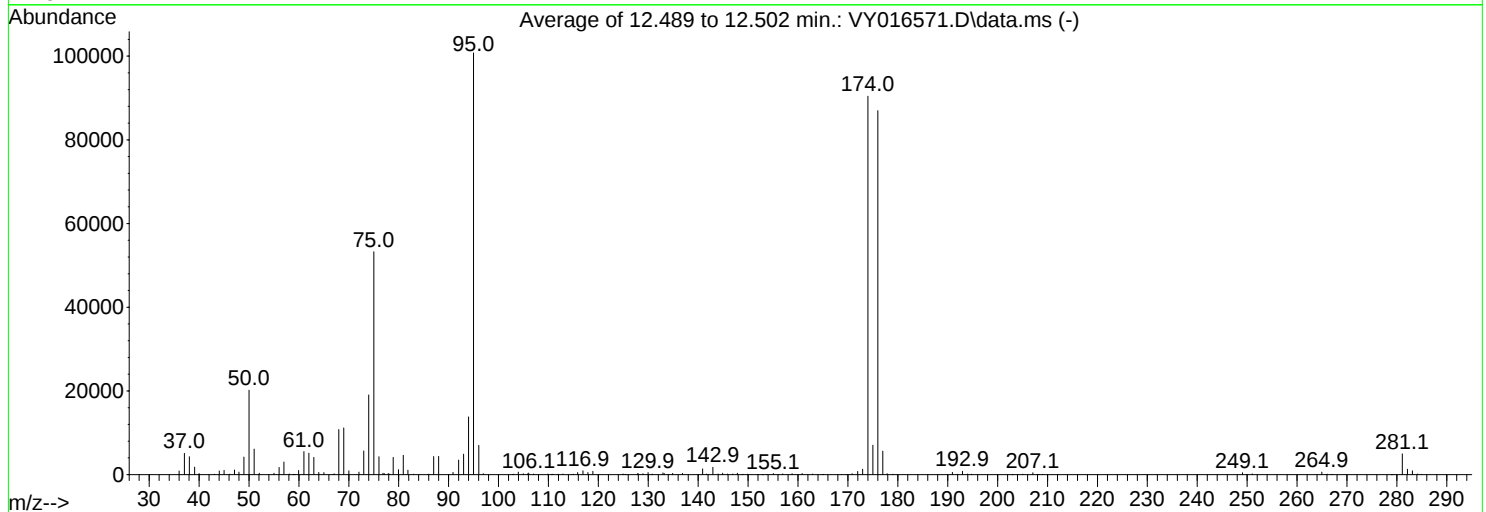


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120423\
 Data File : VY016571.D
 Acq On : 04 Dec 2023 11:30
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120423S.M
 Title : SW846 8260
 Last Update : Tue Dec 05 01:24:25 2023

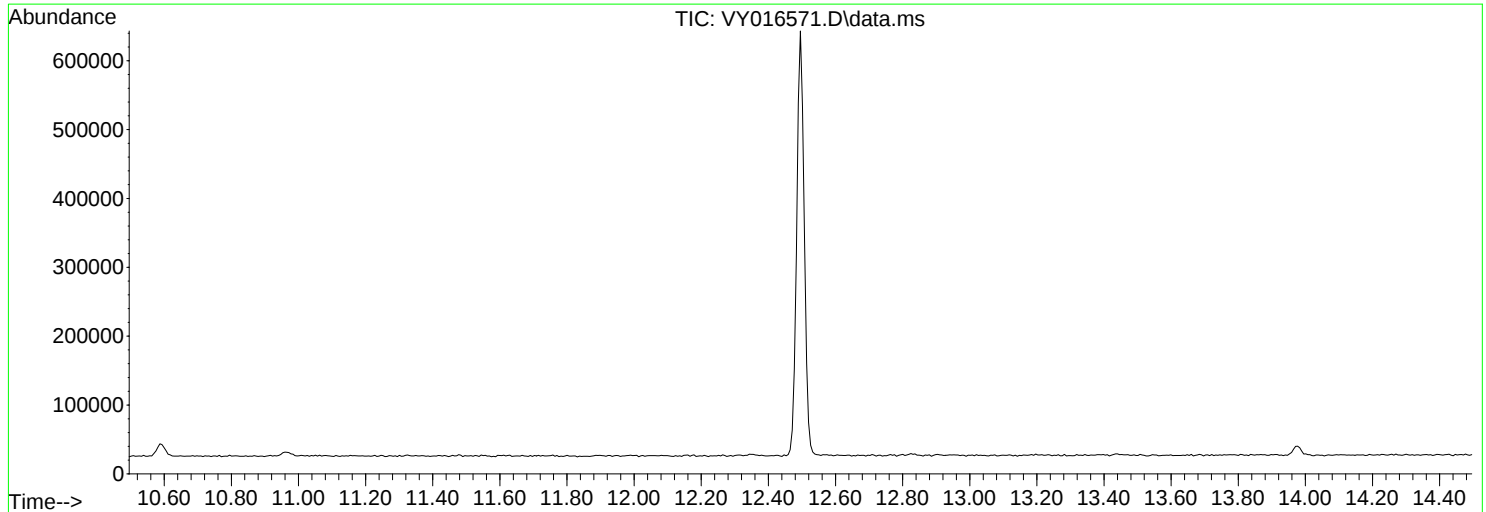

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	20205	PASS
75	95	30	60	52.9	53269	PASS
95	95	100	100	100.0	100789	PASS
96	95	5	9	6.9	6987	PASS
173	174	0.00	2	1.4	1300	PASS
174	95	50	100	89.7	90427	PASS
175	174	5	9	7.8	7046	PASS
176	174	95	101	96.2	86976	PASS
177	176	5	9	6.5	5625	PASS