
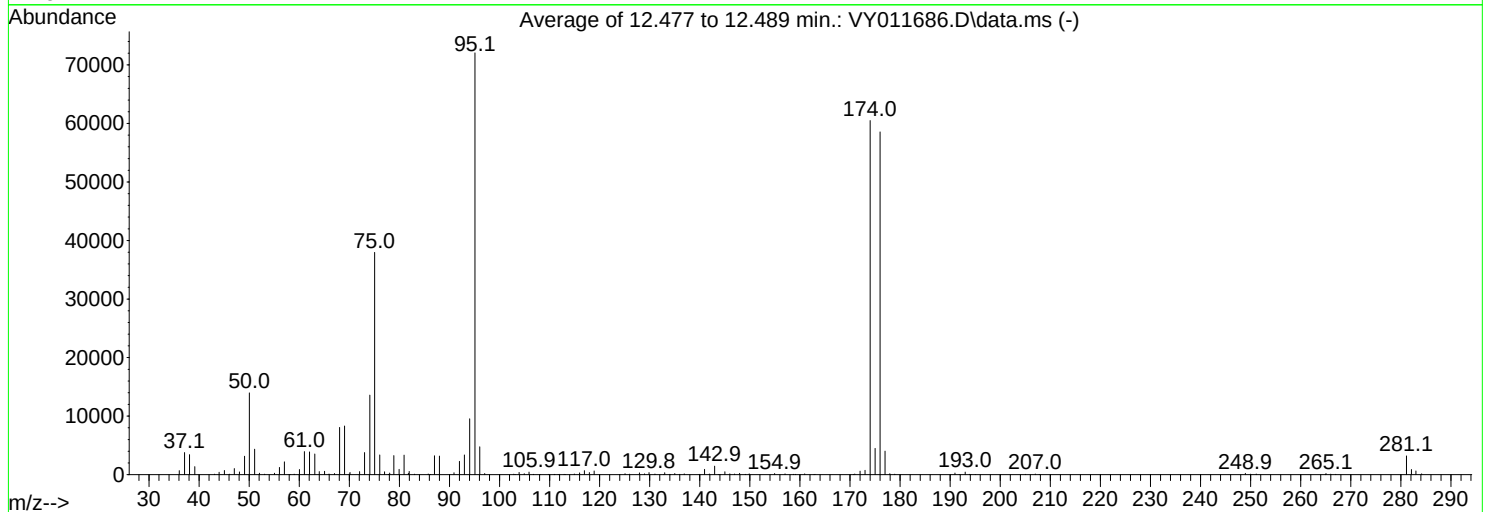


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120522\
Data File : VY011686.D
Acq On : 05 Dec 2022 09:39
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111822S.M
Title : SW846 8260
Last Update : Sat Nov 19 22:37:14 2022

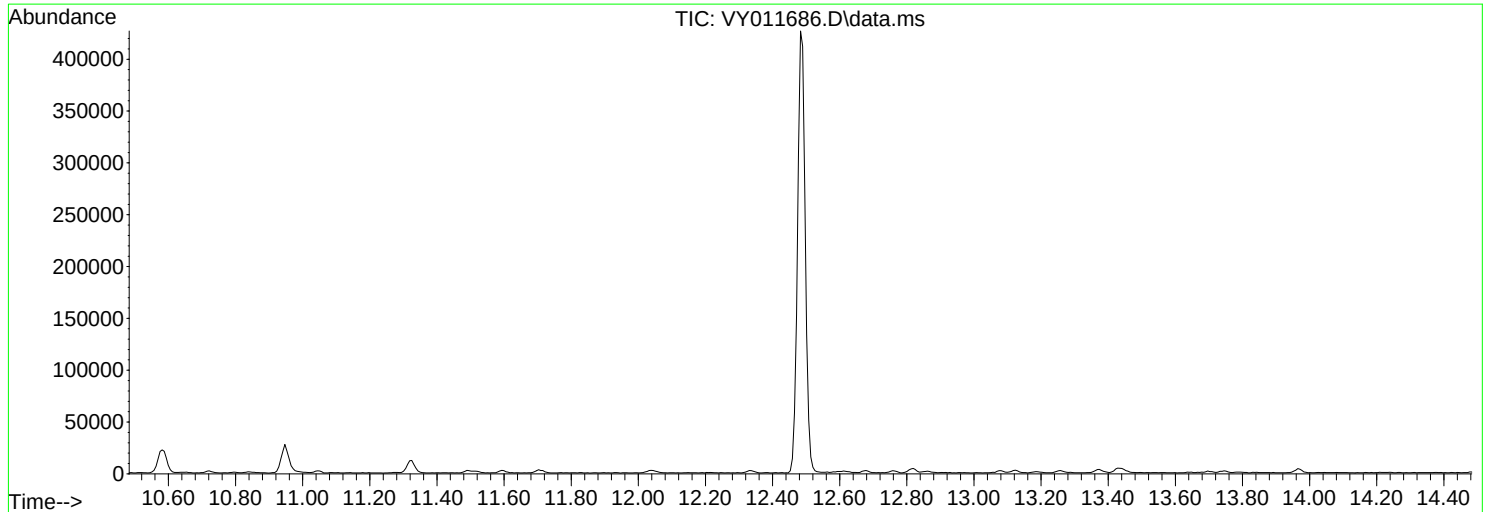

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	13970	PASS
75	95	30	60	52.7	37971	PASS
95	95	100	100	100.0	72061	PASS
96	95	5	9	6.6	4770	PASS
173	174	0.00	2	1.2	739	PASS
174	95	50	100	84.0	60507	PASS
175	174	5	9	7.4	4485	PASS
176	174	95	101	96.8	58541	PASS
177	176	5	9	6.9	4029	PASS