

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120621\
 Data File : VY006966.D
 Acq On : 06 Dec 2021 17:19
 Operator : SY/MD
 Sample : M4887-11
 Misc : 5.49g/10.0mL/MSVOA_Y/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 EX8A6

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 12/14/2021
 Supervised By :Mahesh Dadoda 12/14/2021

Quant Time: Dec 07 00:48:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\SFAMYLEM120321SMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 07 00:43:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.691	114	121259	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.489	117	70672	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.422	152	22386	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.247	65	48854	31.282	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 125.120%			
7) Chloroethane-d5	2.765	69	33224	27.120	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 108.480%			
11) 1,1-Dichloroethene-d2	3.844	63	47961	14.772	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery = 59.080%			
21) 2-Butanone-d5	6.887	46	18589	30.818	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 61.640%			
24) Chloroform-d	7.472	84	65963	21.828	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 87.320%			
26) 1,2-Dichloroethane-d4	8.136	65	41619	22.944	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 91.760%			
32) Benzene-d6	8.106	84	119939	31.949	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 127.800%			
36) 1,2-Dichloropropane-d6	9.118	67	40961	34.727	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 138.920%#			
41) Toluene-d8	10.179	98	82252	23.393	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 93.560%			
43) trans-1,3-Dichloroprop...	10.435	79	14262	24.999	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 100.000%			
47) 2-Hexanone-d5	10.788	63	13209	48.386	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 96.780%			
56) 1,1,2,2-Tetrachloroeth...	12.556	84	27574	28.060	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 112.240%			
66) 1,2-Dichlorobenzene-d4	13.721	152	12426	17.021	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 68.080%#			
Target Compounds					Qvalue	
13) Acetone	3.924	43	2269m	4.105	ug/L	
46) Tetrachloroethene	10.715	164	164232	167.499	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120621\
Data File : VY006966.D
Acq On : 06 Dec 2021 17:19
Operator : SY/MD
Sample : M4887-11
Misc : 5.49g/10.0mL/MSVOA_Y/SOIL
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_Y
ClientSampleId :
EX8A6

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 12/14/2021
Supervised By : Mahesh Dadoda 12/14/2021


Quant Time: Dec 07 00:48:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\SFAMYL120321SMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 07 00:43:47 2021
Response via : Initial Calibration

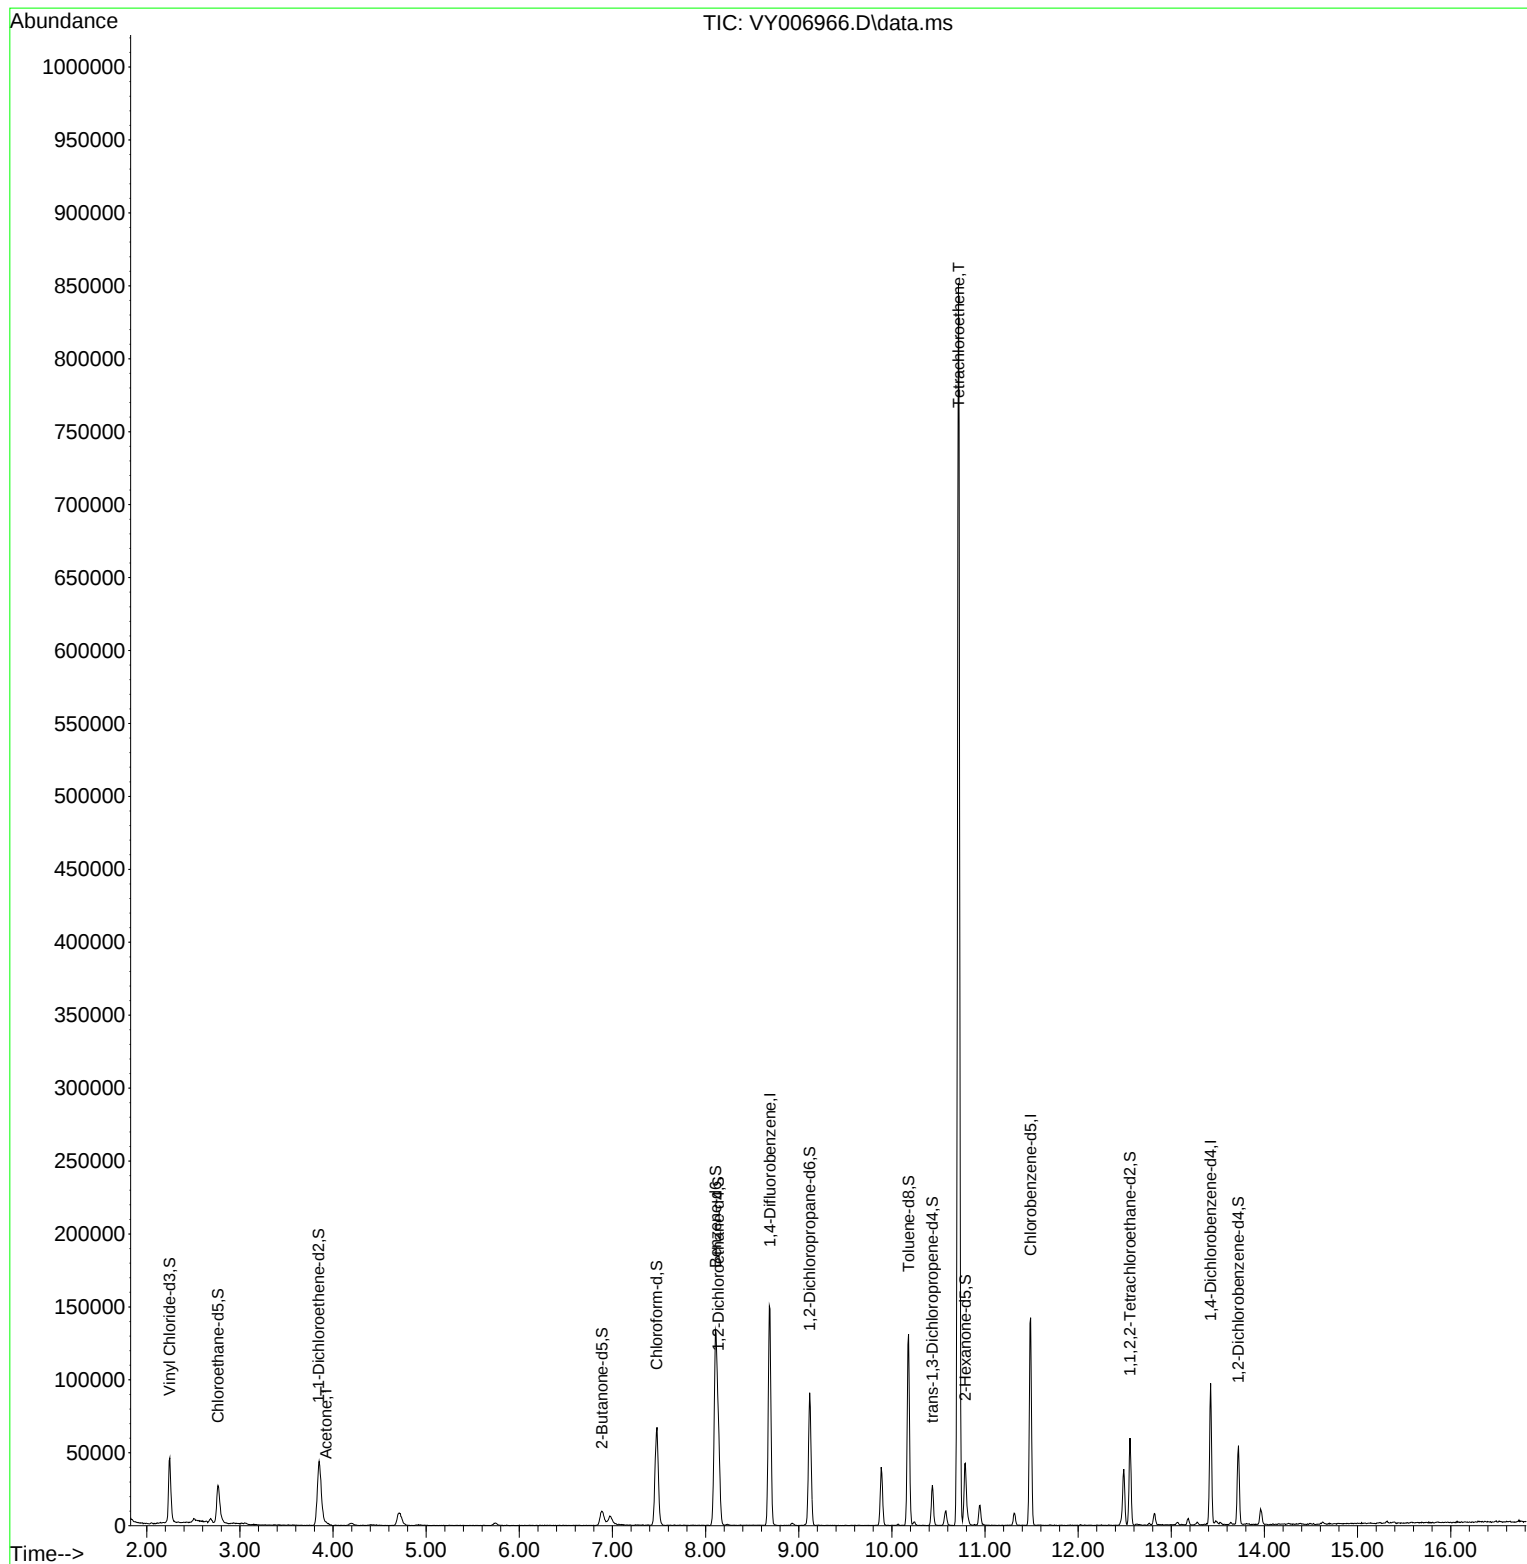

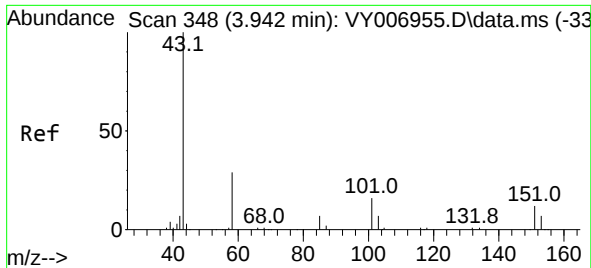

#13
Acetone
Concen: 4.105 ug/L m
RT: 3.924 min Scan# 34
Delta R.T. -0.018 min
Lab File: VY006966.D
Acq: 06 Dec 2021 17:19




Instrument :
MSVOA_Y
ClientSampleId :
EX8A6

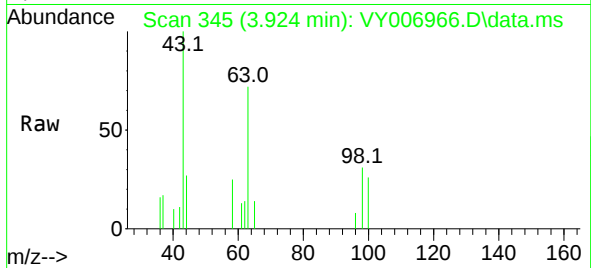


Tgt Ion: 43 Resp: 2269
Ion Ratio Lower Upper
43 100
58 1.9 0.0 60.8

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 12/14/2021
Supervised By :Mahesh Dadoda 12/14/2021

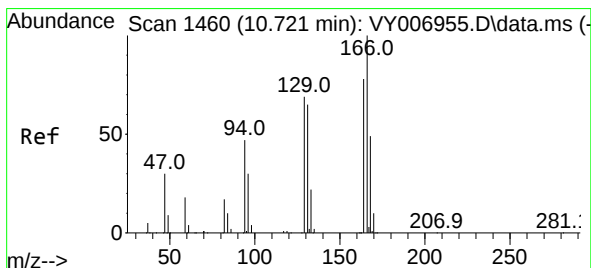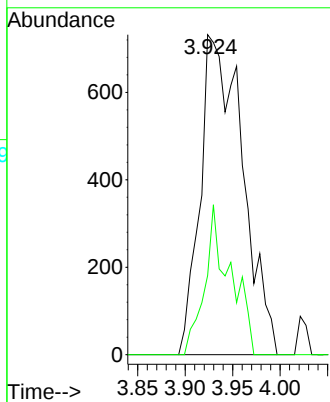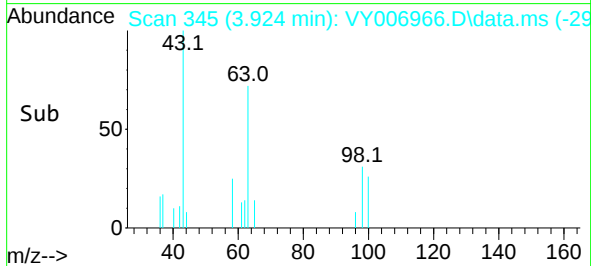

#46
Tetrachloroethene
Concen: 167.499 ug/L
RT: 10.715 min Scan# 1459
Delta R.T. -0.006 min
Lab File: VY006966.D
Acq: 06 Dec 2021 17:19

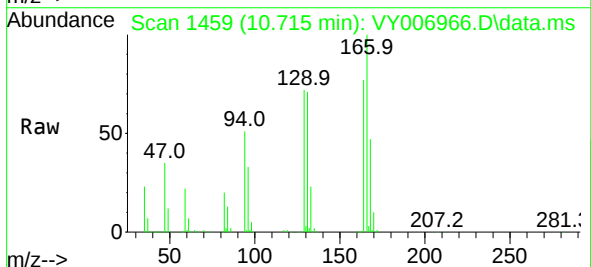

Tgt Ion:164 Resp: 164232
Ion Ratio Lower Upper
164 100
129 94.4 62.1 115.3
131 92.5 61.0 113.2
166 130.4 90.4 168.0

