

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120623\
 Data File : VY016615.D
 Acq On : 06 Dec 2023 14:57
 Operator : SY/MD
 Sample : 05599-05RE
 Misc : 4.71g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 LKWD-BACKFILL-03RE

Quant Time: Dec 07 00:33:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120423S.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 05 01:24:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.807	168	123721	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.704	114	201408	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.508	117	196022	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.440	152	95597	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.155	65	79138	69.206	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	138.420%
35) Dibromofluoromethane	7.734	113	63241	52.176	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	104.360%
50) Toluene-d8	10.197	98	231134	50.414	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	100.820%
62) 4-Bromofluorobenzene	12.496	95	83798	55.580	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	111.160%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120623\
Data File : VY016615.D
Acq On : 06 Dec 2023 14:57
Operator : SY/MD
Sample : 05599-05RE
Misc : 4.71g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
LKWD-BACKFILL-03RE


Quant Time: Dec 07 00:33:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120423S.M
Quant Title : SW846 8260
QLast Update : Tue Dec 05 01:24:25 2023
Response via : Initial Calibration

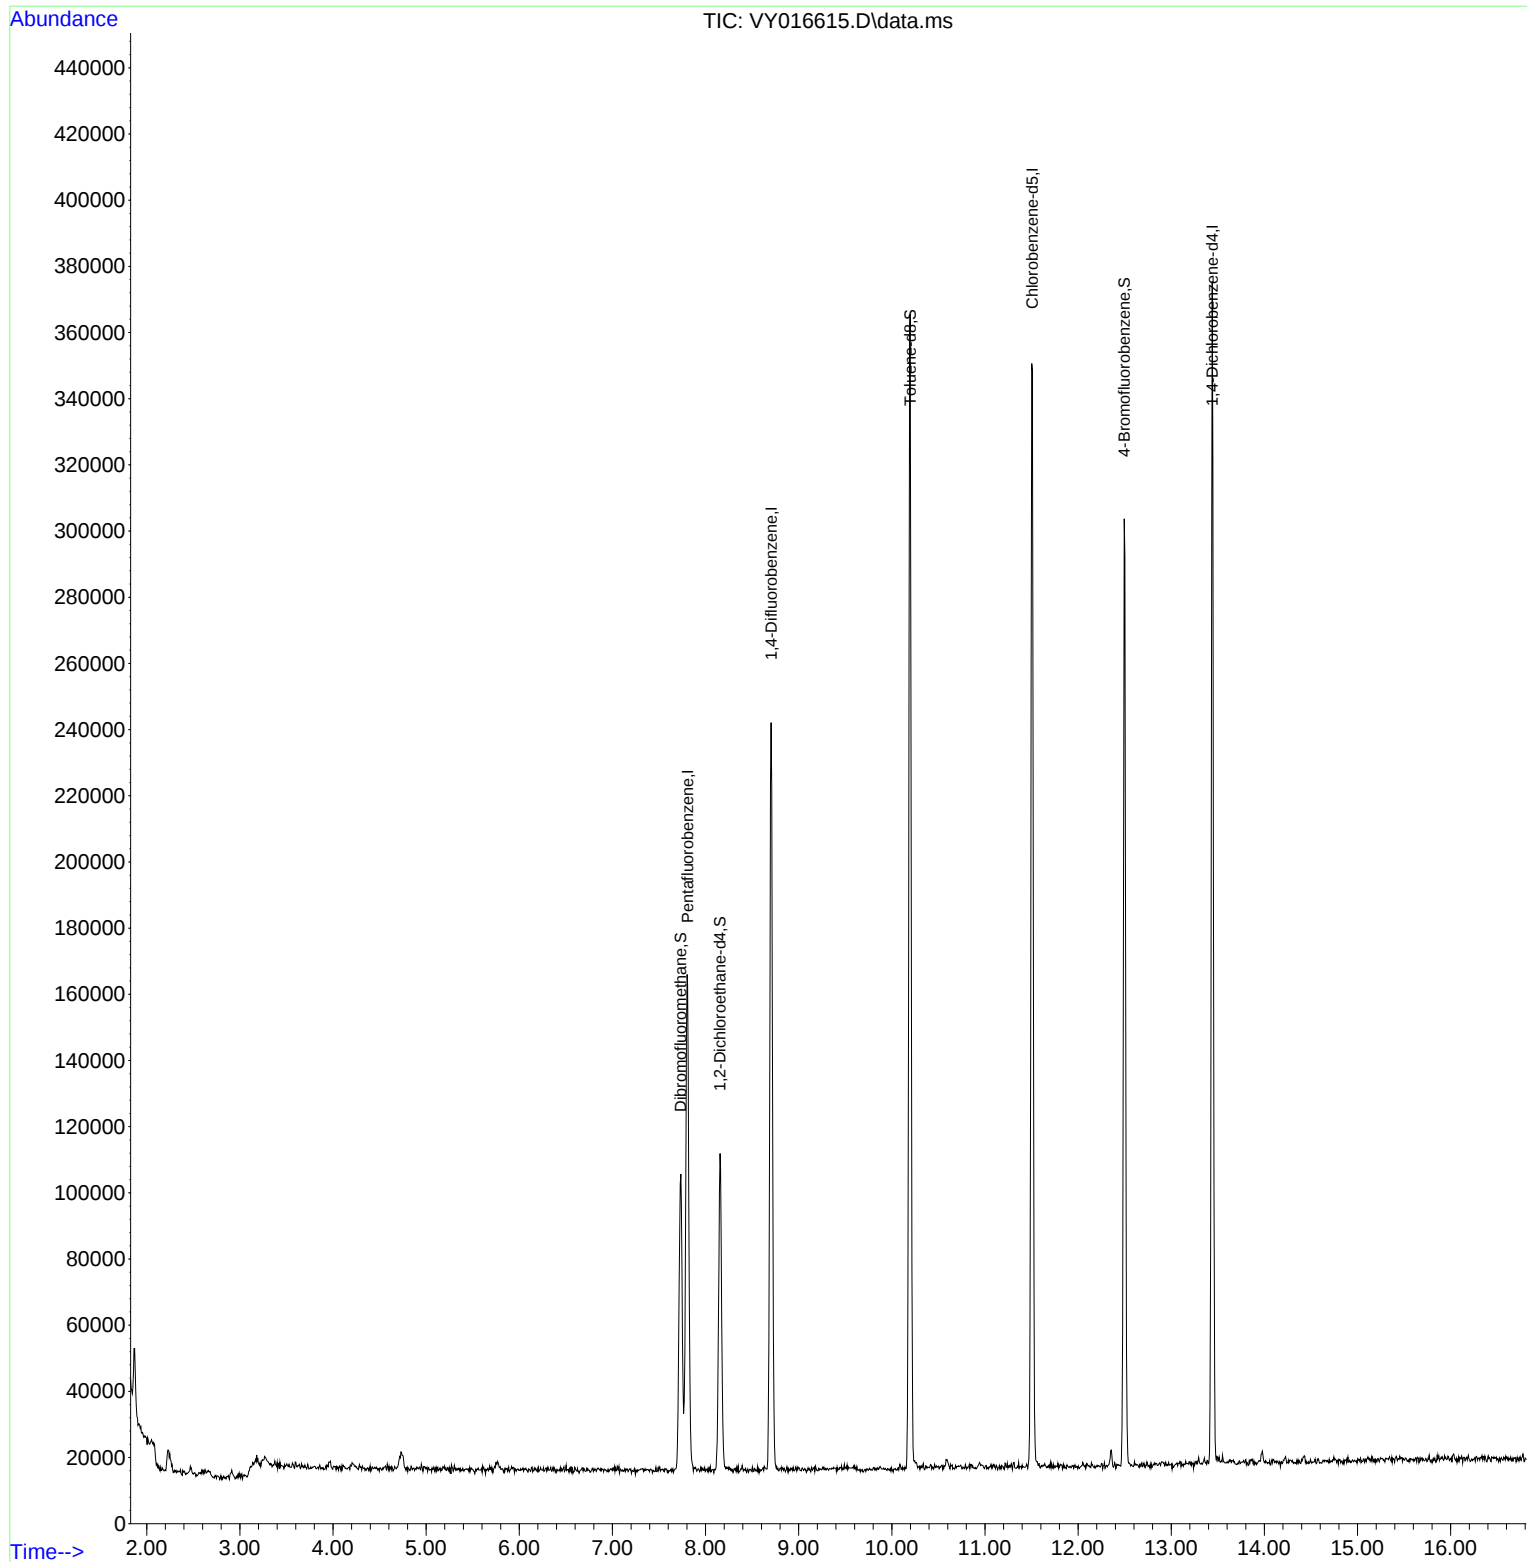



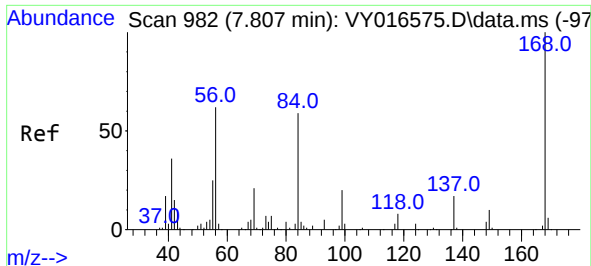


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.807 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY016615.D
Acq: 06 Dec 2023 14:57

Instrument :
MSVOA_Y
ClientSampleId :
LKWD-BACKFILL-03RE



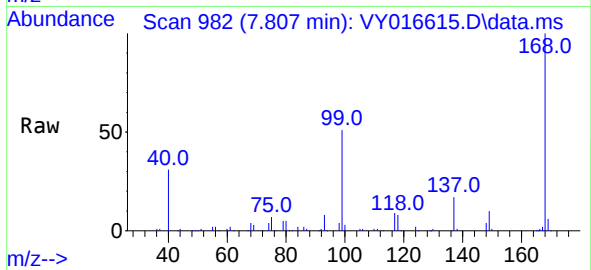



Tgt Ion:168 Resp: 123721
Ion Ratio Lower Upper
168 100
99 51.5 43.4 65.0

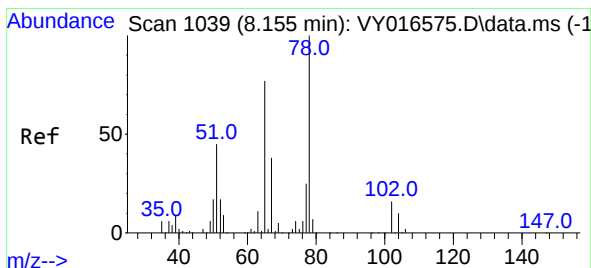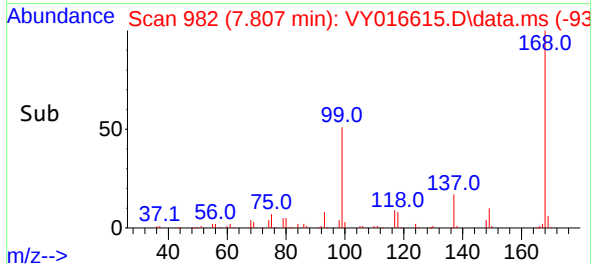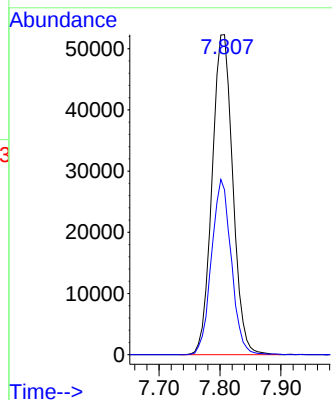

#33
1,2-Dichloroethane-d4
Concen: 69.206 ug/l
RT: 8.155 min Scan# 1039
Delta R.T. 0.000 min
Lab File: VY016615.D
Acq: 06 Dec 2023 14:57

Tgt Ion: 65 Resp: 79138
Ion Ratio Lower Upper
65 100
67 49.4 0.0 101.8

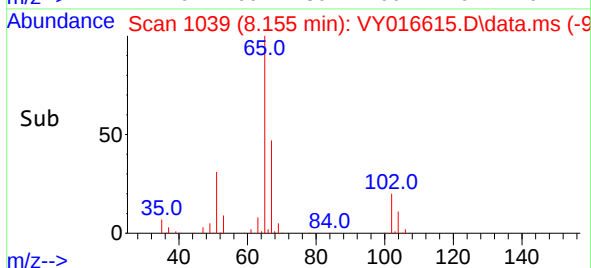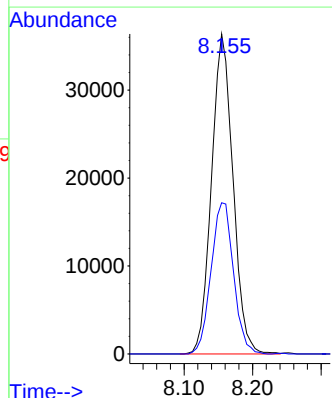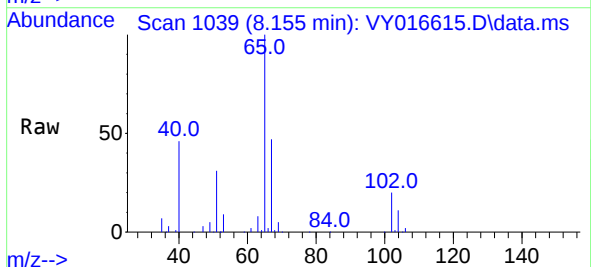

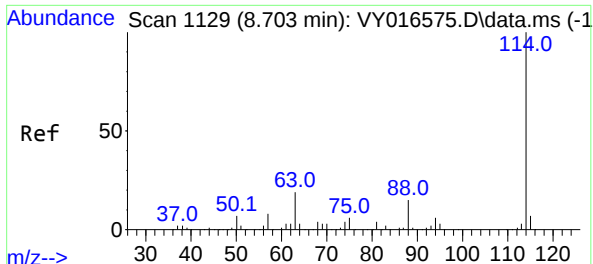

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.704 min Scan# 1129

Delta R.T. 0.000 min

Lab File: VY016615.D

Acq: 06 Dec 2023 14:57

Instrument :

MSVOA_Y

ClientSampleId :

LKWD-BACKFILL-03RE





Tgt Ion:114 Resp: 201408

Ion Ratio Lower Upper

114 100

63 17.5 0.0 42.4

88 15.9 0.0 30.6

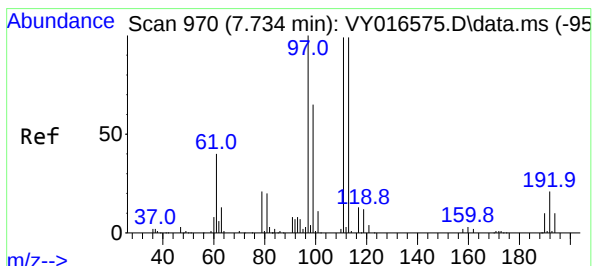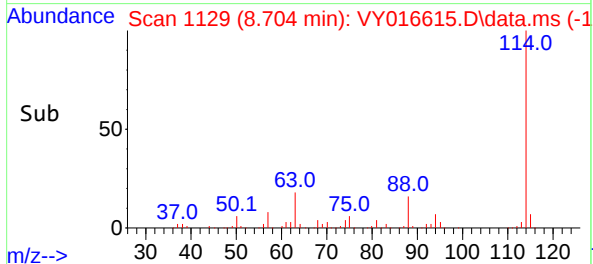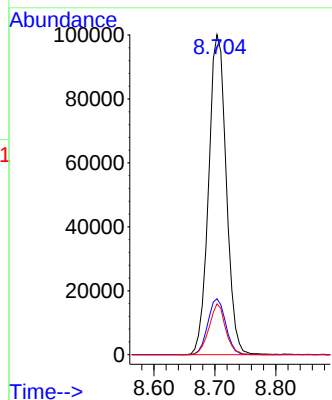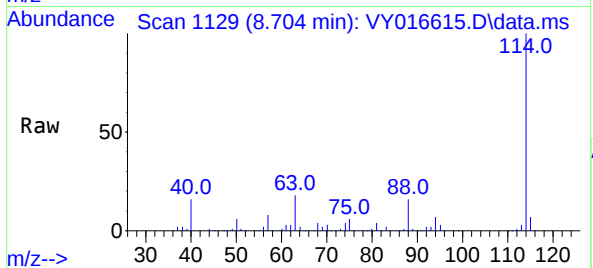

#35

Dibromofluoromethane

Concen: 52.176 ug/l

RT: 7.734 min Scan# 970

Delta R.T. 0.000 min

Lab File: VY016615.D

Acq: 06 Dec 2023 14:57




Tgt Ion:113 Resp: 63241


Ion Ratio Lower Upper

113 100

111 103.5 81.3 121.9

192 22.3 16.9 25.3


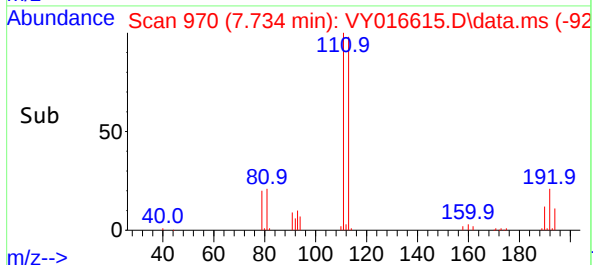
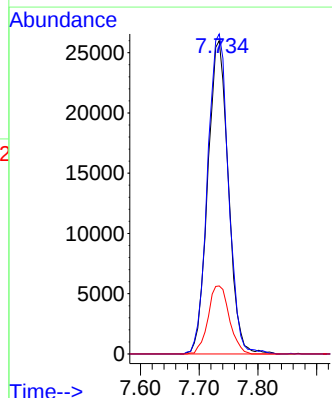
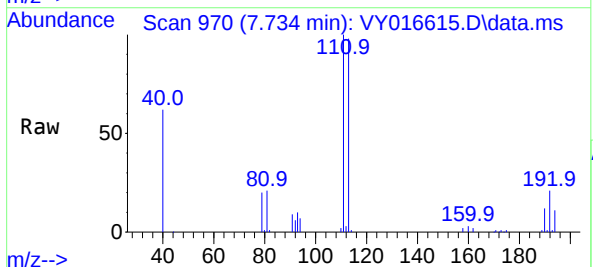


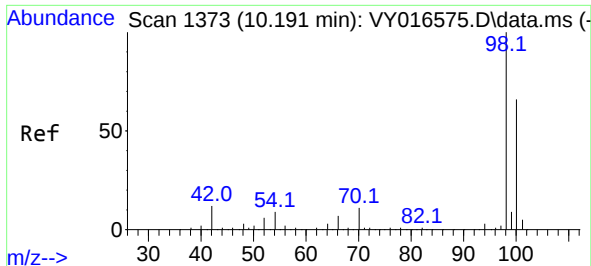

#50
Toluene-d8
Concen: 50.414 ug/l
RT: 10.197 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY016615.D
Acq: 06 Dec 2023 14:57




Instrument :
MSVOA_Y
ClientSampleId :
LKWD-BACKFILL-03RE


Tgt Ion: 98 Resp: 231134
Ion Ratio Lower Upper
98 100
100 65.5 50.1 75.1

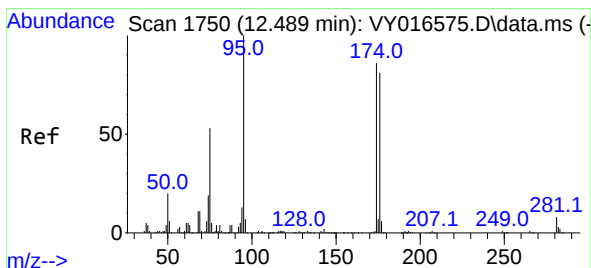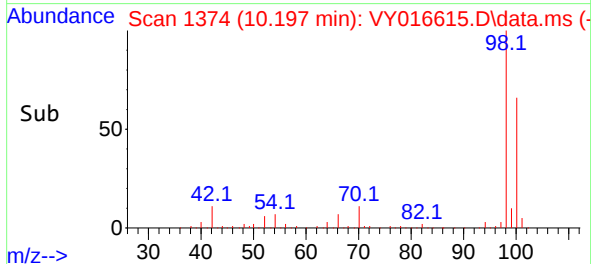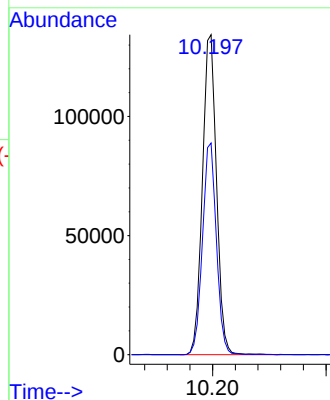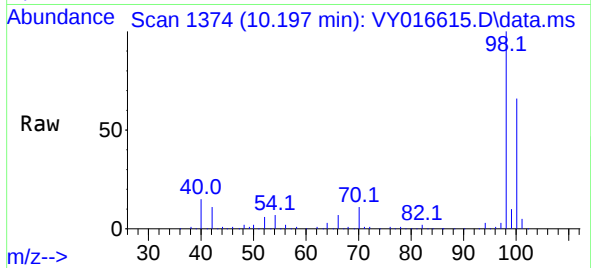

#62
4-Bromofluorobenzene
Concen: 55.580 ug/l
RT: 12.496 min Scan# 1751
Delta R.T. 0.006 min
Lab File: VY016615.D
Acq: 06 Dec 2023 14:57

Tgt Ion: 95 Resp: 83798
Ion Ratio Lower Upper
95 100
174 96.3 0.0 178.2
176 92.3 0.0 173.8


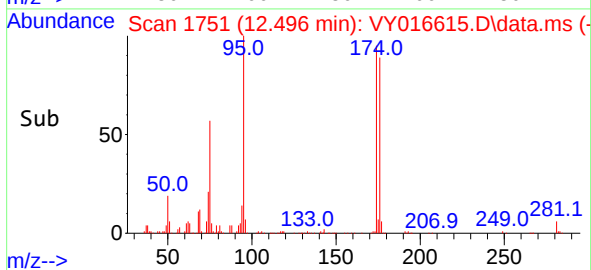
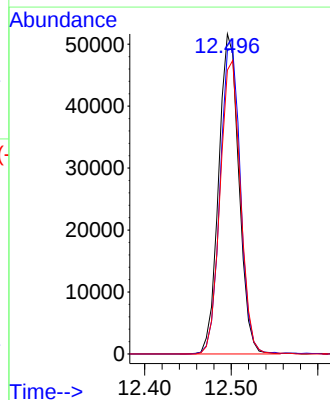
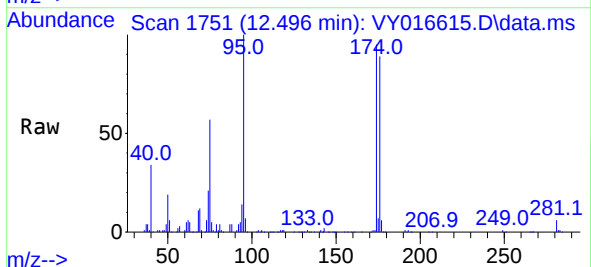


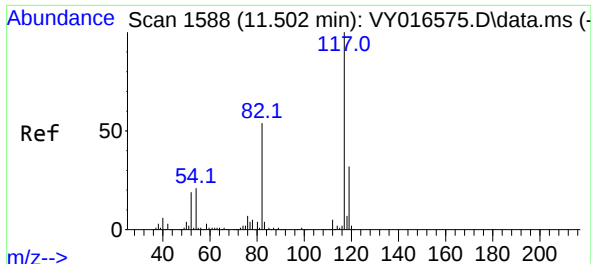

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.508 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY016615.D
Acq: 06 Dec 2023 14:57

Instrument :
MSVOA_Y
ClientSampleId :
LKWD-BACKFILL-03RE

Tgt Ion:117 Resp: 196022
Ion Ratio Lower Upper
117 100
82 51.9 43.4 65.0
119 32.4 26.3 39.5

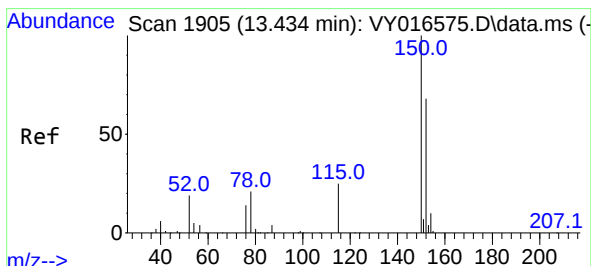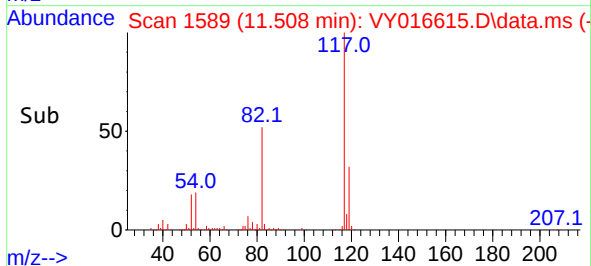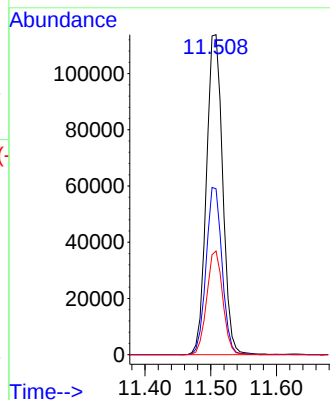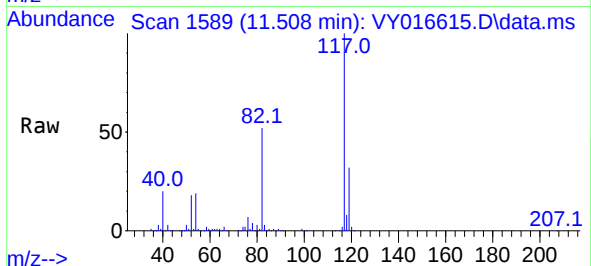

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.440 min Scan# 1906
Delta R.T. 0.006 min
Lab File: VY016615.D
Acq: 06 Dec 2023 14:57

Tgt Ion:152 Resp: 95597
Ion Ratio Lower Upper
152 100
115 56.0 28.8 86.5
150 155.3 0.0 348.8

